

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR082118\
Quantitation Report (QT Reviewed)


Data File : VR025623.D
Acq On : 21 Aug 2018 12:04
Operator : SY/MD
Sample : VSTD0.581
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD0.581

Manual Integrations
APPROVED

MMDadoda
8/22/2018 10:49:49 AM

Quant Time: Aug 21 16:48:38 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR082118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 21 16:35:04 2018
Response via : Initial Calibration

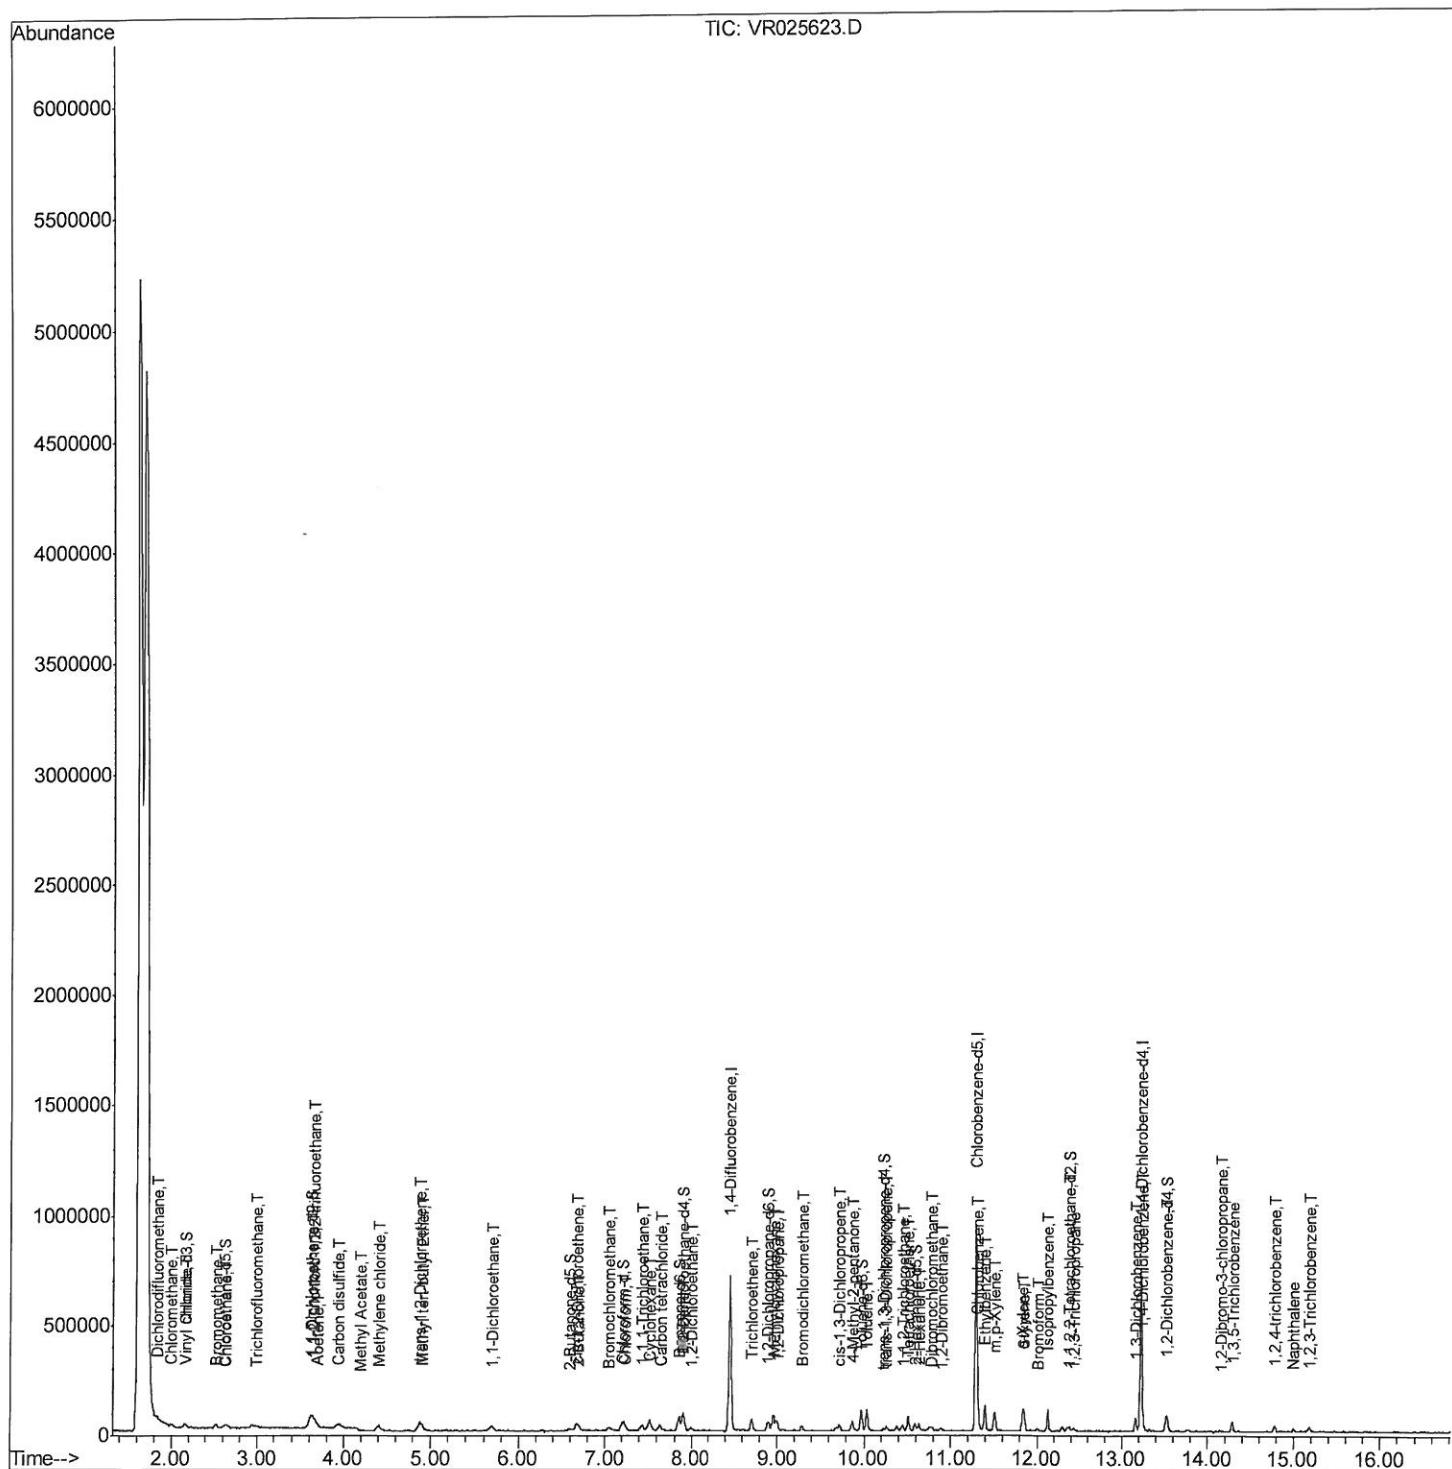

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR082118\
Quantitation Report (Qedit)




Data File : VR025623.D
Acq On : 21 Aug 2018 12:04
Operator : SY/MD
Sample : VSTD0.581
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD0.581

Manual Integrations
APPROVED

MMDadoda
8/22/2018 10:49:49 AM

Quant Time: Aug 21 16:35:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR082118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 21 16:35:04 2018
Response via : Initial Calibration

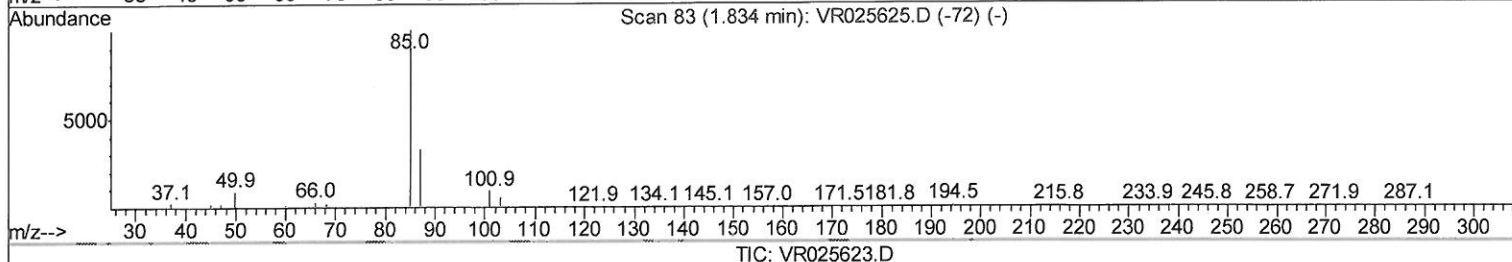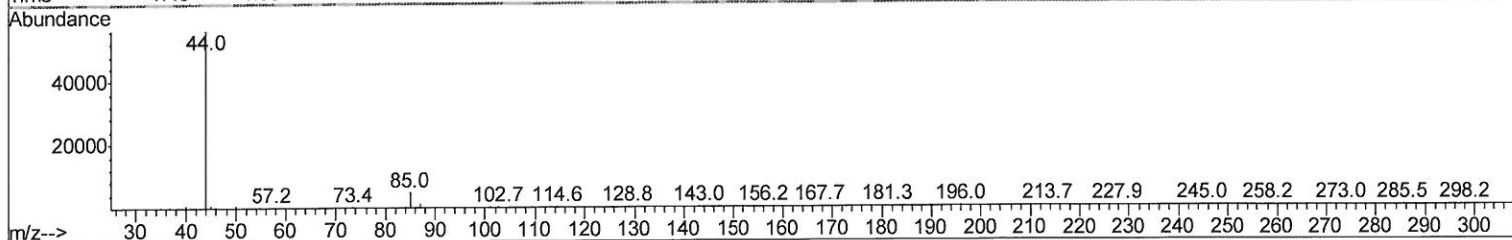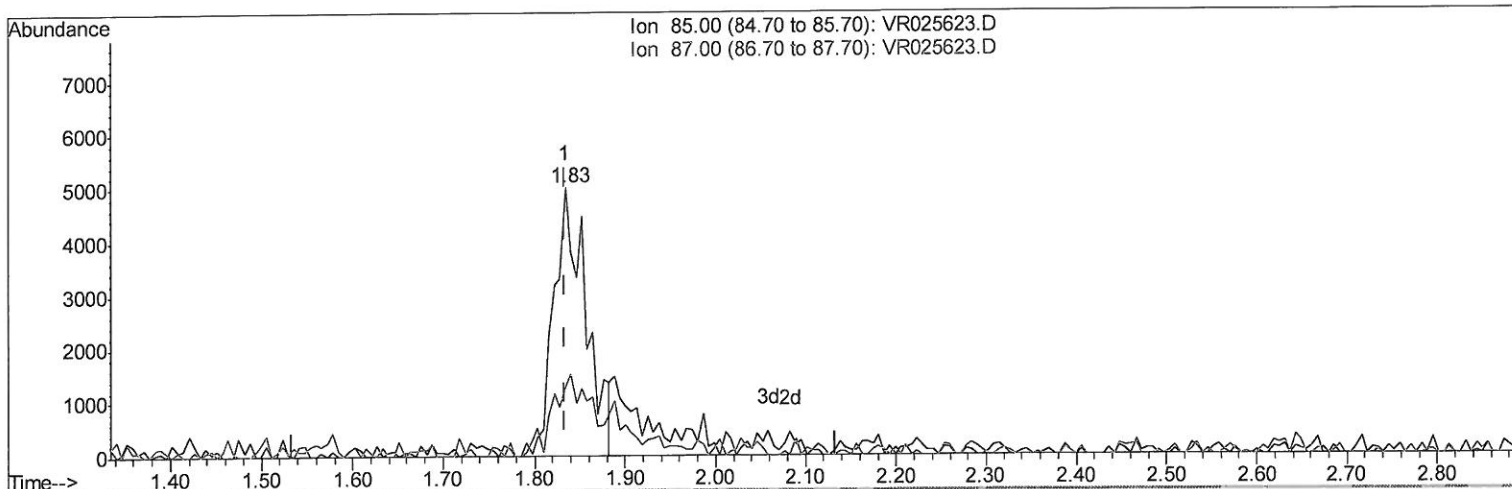

TIC: VR025623.D

(2) Dichlorodifluoromethane (T)

1.834min (+0.000) 0.38ug/L

response 12571

Ion	Exp%	Act%
85.00	100	100
87.00	29.40	35.18
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR082118\
Quantitation Report (Qedit)




Data File : VR025623.D
Acq On : 21 Aug 2018 12:04
Operator : SY/MD
Sample : VSTD0.581
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD0.581

Manual Integrations
APPROVED

MMDadoda
8/22/2018 10:49:49 AM

Quant Time: Aug 21 16:35:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR082118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 21 16:35:04 2018
Response via : Initial Calibration

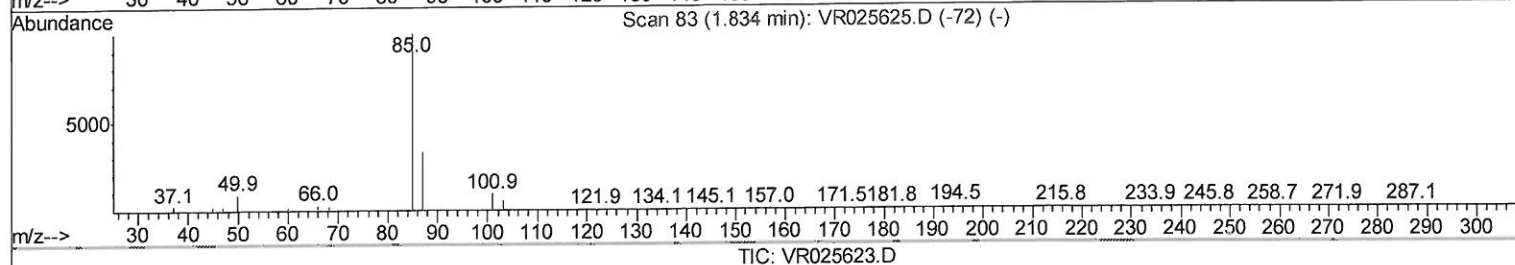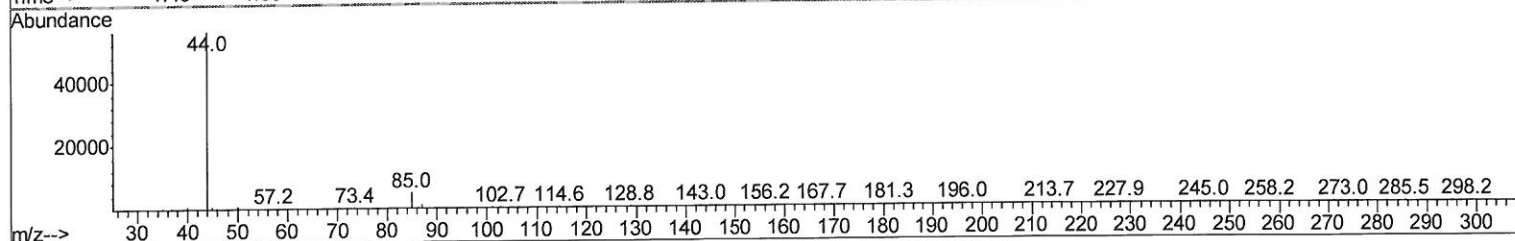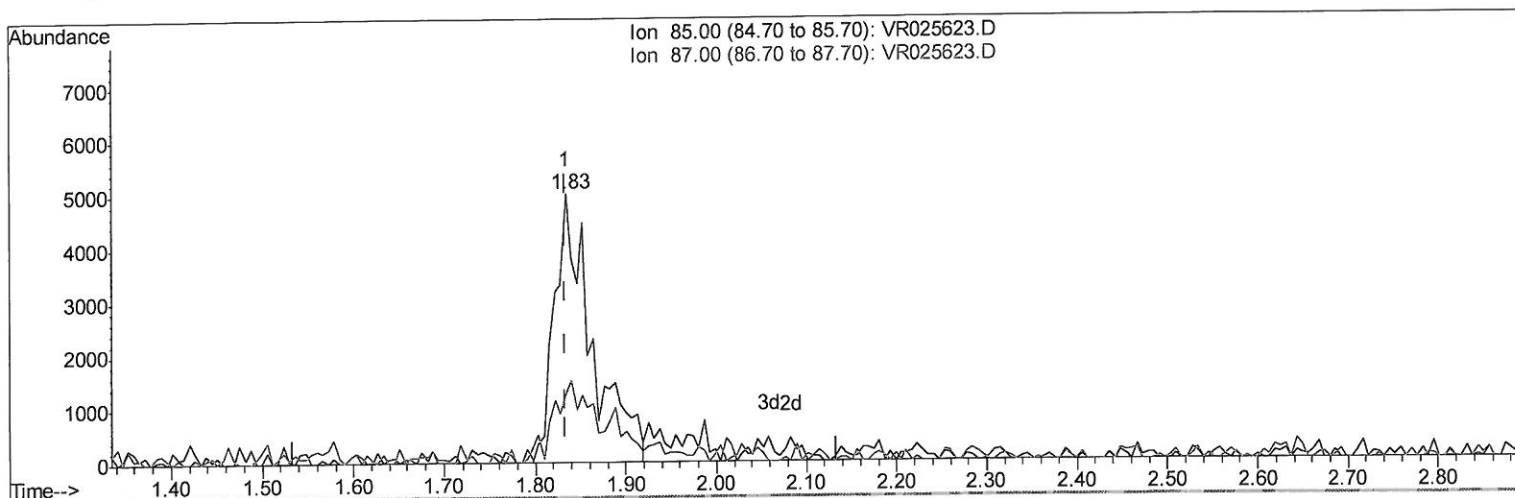

(2) Dichlorodifluoromethane (T)

1.834min (+0.000) 0.44ug/L m

response 14491

Ion	Exp%	Act%
85.00	100	100
87.00	29.40	30.52
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR082118\
Quantitation Report (Qedit)




Data File : VR025623.D
Acq On : 21 Aug 2018 12:04
Operator : SY/MD
Sample : VSTD0.581
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD0.581

Manual Integrations
APPROVED

MMDadoda
8/22/2018 10:49:49 AM

Quant Time: Aug 21 16:35:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR082118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 21 16:35:04 2018
Response via : Initial Calibration

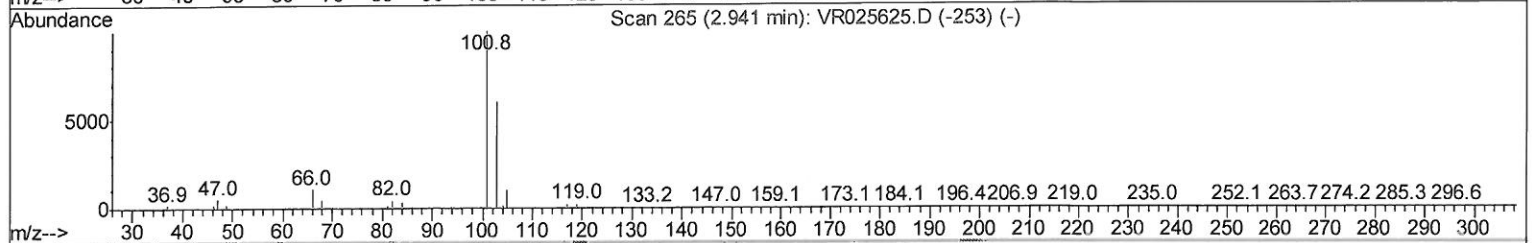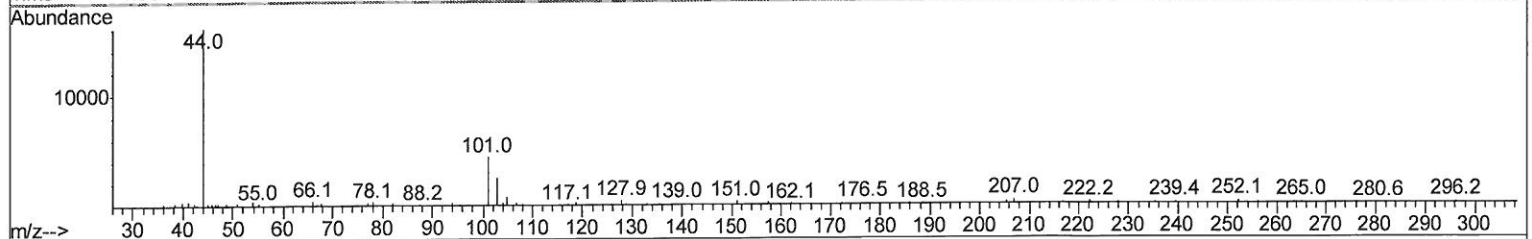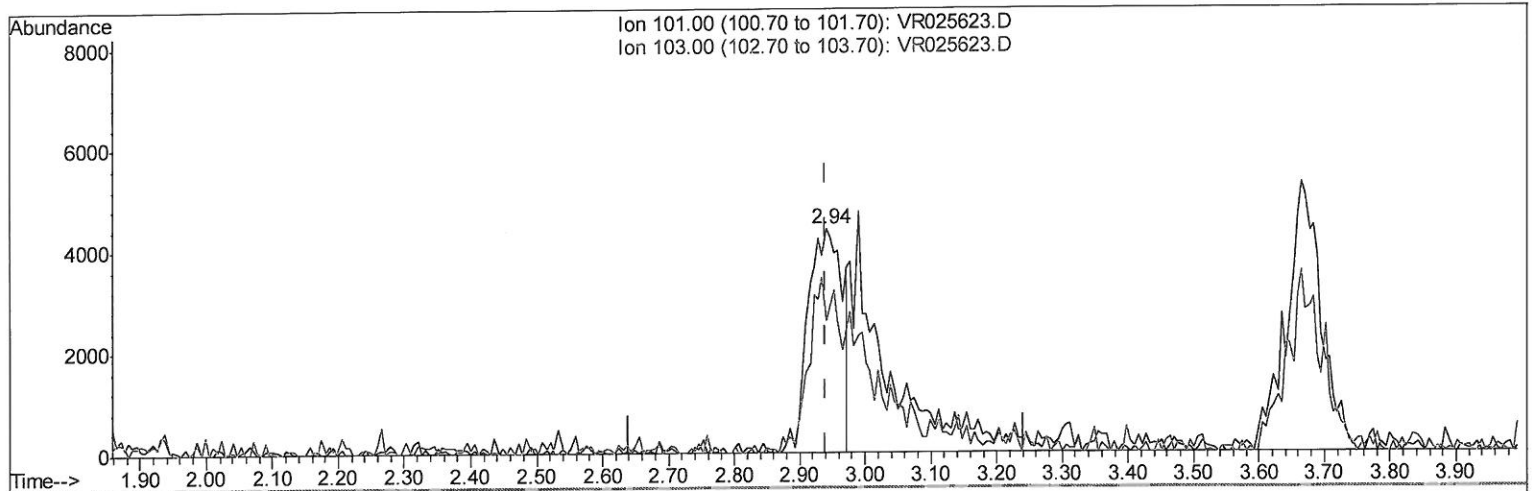

TIC: VR025623.D

(9) Trichlorofluoromethane (T)

2.941min (+0.000) 0.24ug/L

response 16028

Ion	Exp%	Act%
101.00	100	100
103.00	20.50	63.47#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR082118\
Quantitation Report (Qedit)




Data File : VR025623.D
Acq On : 21 Aug 2018 12:04
Operator : SY/MD
Sample : VSTD0.581
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampled :
VSTD0.581

Manual Integrations
APPROVED

MMDadoda
8/22/2018 10:49:49 AM

Quant Time: Aug 21 16:35:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR082118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 21 16:35:04 2018
Response via : Initial Calibration

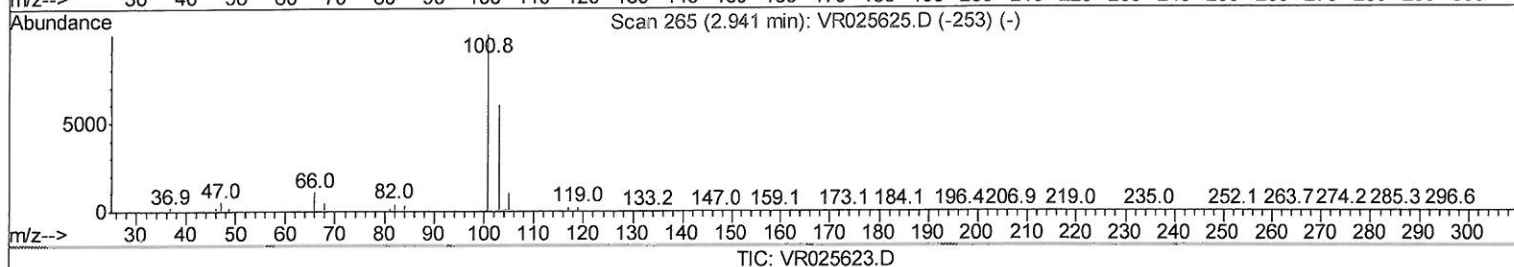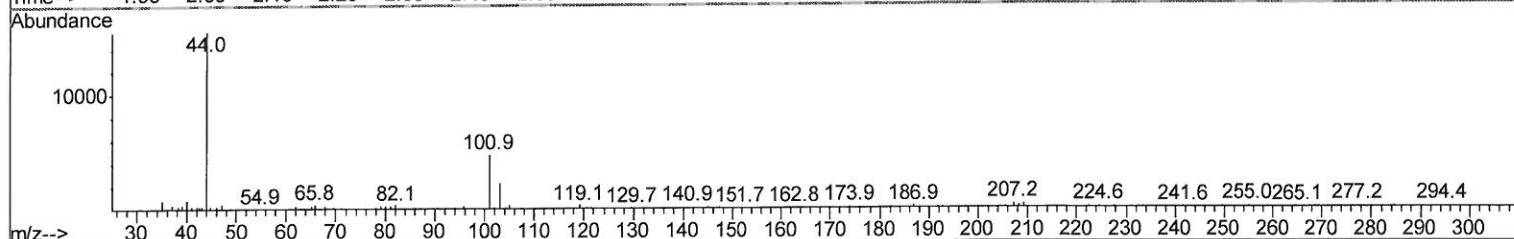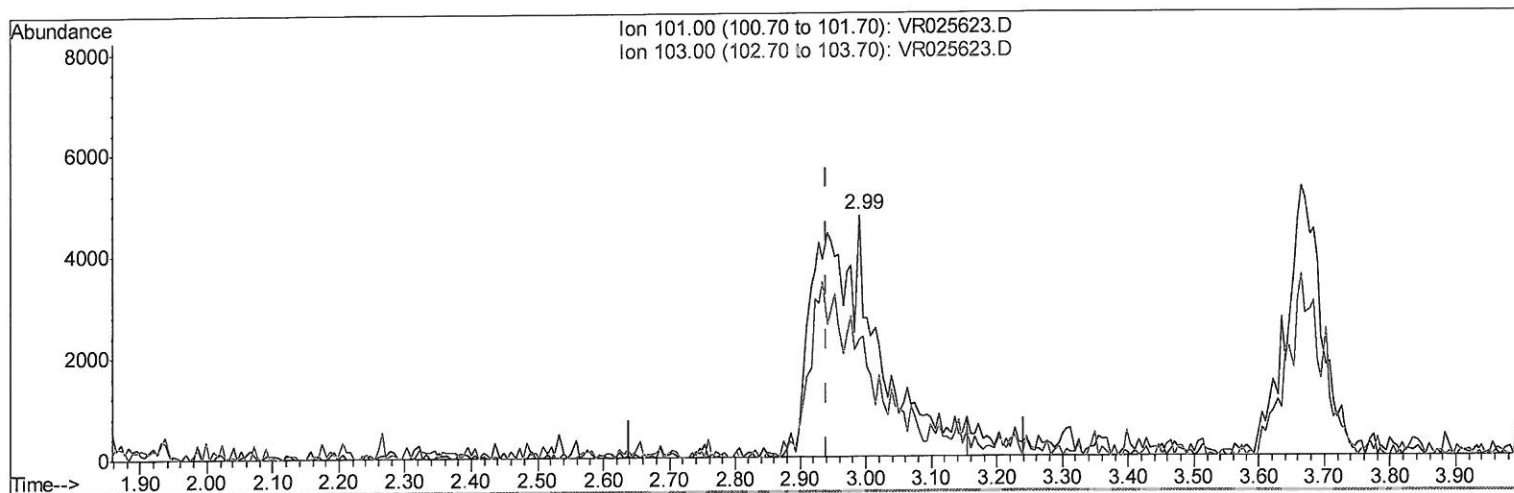

(9) Trichlorofluoromethane (T)

2.990min (+0.049) 0.48ug/L m

response 31577

Ion	Exp%	Act%
101.00	100	100
103.00	20.50	32.22#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR082118\
Quantitation Report (Qedit)




Data File : VR025623.D
Acq On : 21 Aug 2018 12:04
Operator : SY/MD
Sample : VSTD0.581
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD0.581

Manual Integrations
APPROVED

MMDadoda
8/22/2018 10:49:49 AM

Quant Time: Aug 21 16:35:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR082118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 21 16:35:04 2018
Response via : Initial Calibration

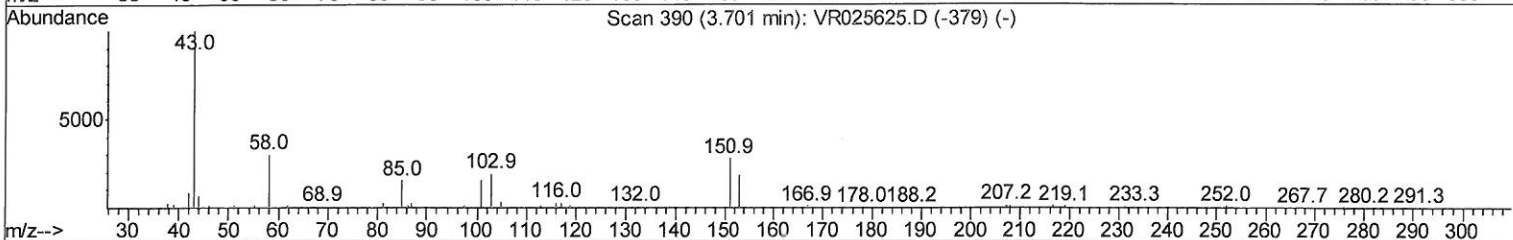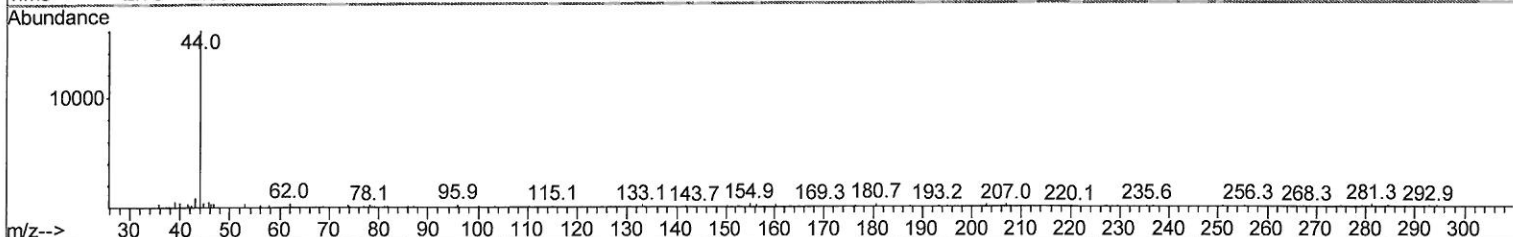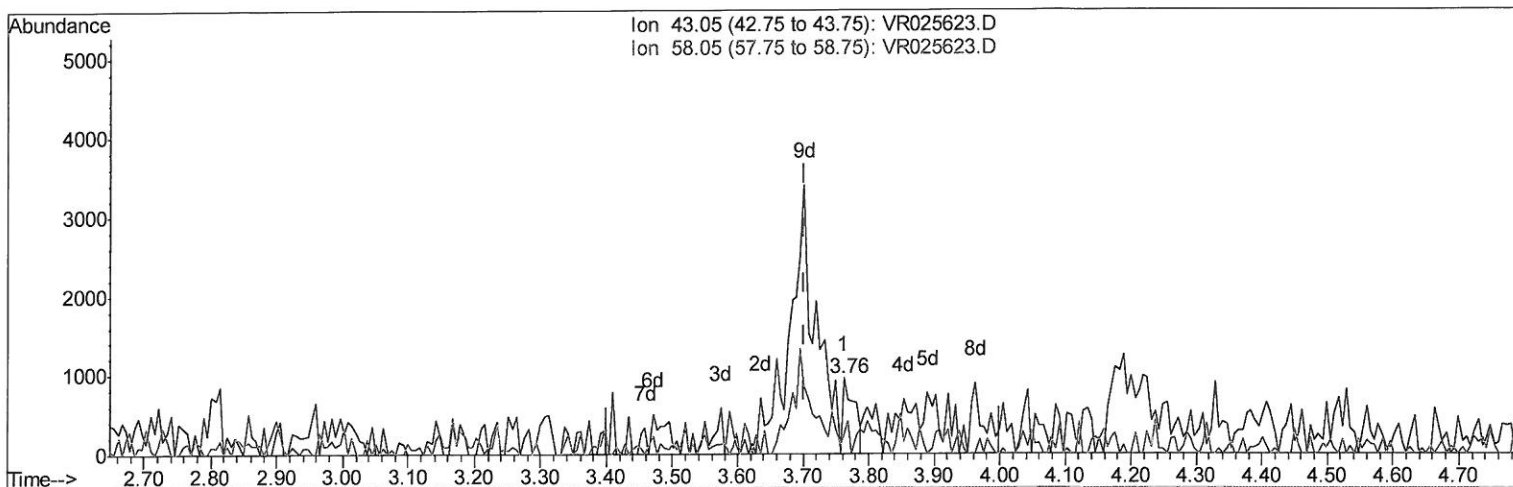

TIC: VR025623.D

(13) Acetone (T)

3.762min (+0.061) 0.32ug/L

response 1201

Ion	Exp%	Act%
43.05	100	100
58.05	31.70	29.64
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR082118\
Quantitation Report (Qedit)




Data File : VR025623.D
Acq On : 21 Aug 2018 12:04
Operator : SY/MD
Sample : VSTD0.581
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD0.581

Manual Integrations
APPROVED

MMDadoda
8/22/2018 10:49:49 AM

Quant Time: Aug 21 16:35:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR082118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 21 16:35:04 2018
Response via : Initial Calibration

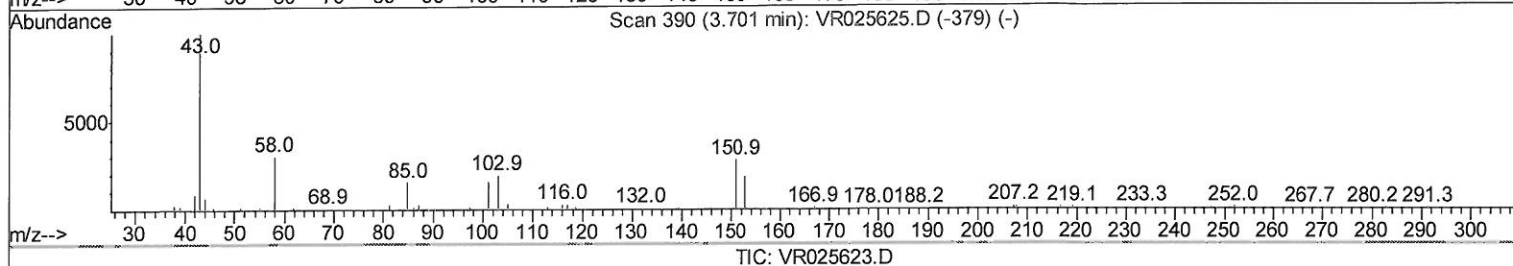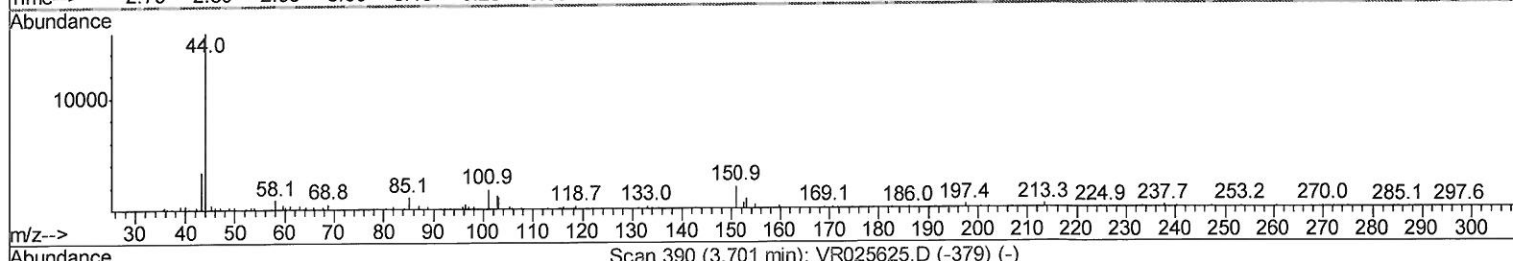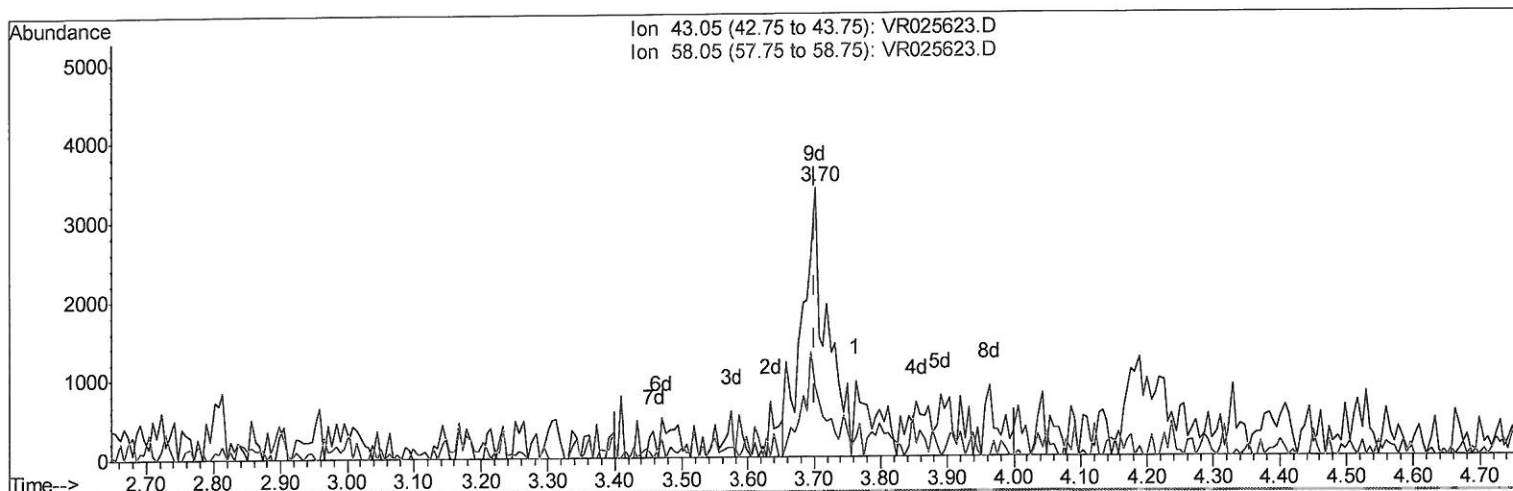

(13) Acetone (T)

3.702min (+0.000) 2.29ug/L m

08/22/18 SY

response 8679

Ion	Exp%	Act%
43.05	100	100
58.05	31.70	4.10
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR082118\
Quantitation Report (Qedit)




Data File : VR025623.D
Acq On : 21 Aug 2018 12:04
Operator : SY/MD
Sample : VSTD0.581
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD0.581

Manual Integrations
APPROVED

MMDadoda
8/22/2018 10:49:49 AM

Quant Time: Aug 21 16:35:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR082118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 21 16:35:04 2018
Response via : Initial Calibration

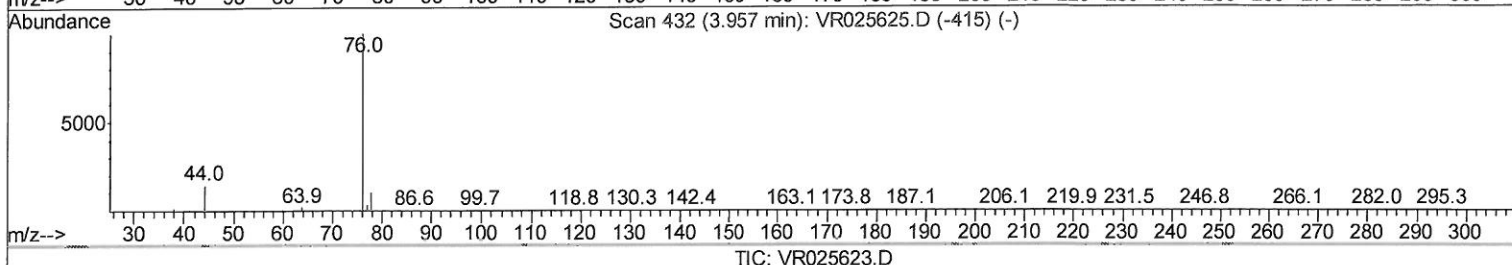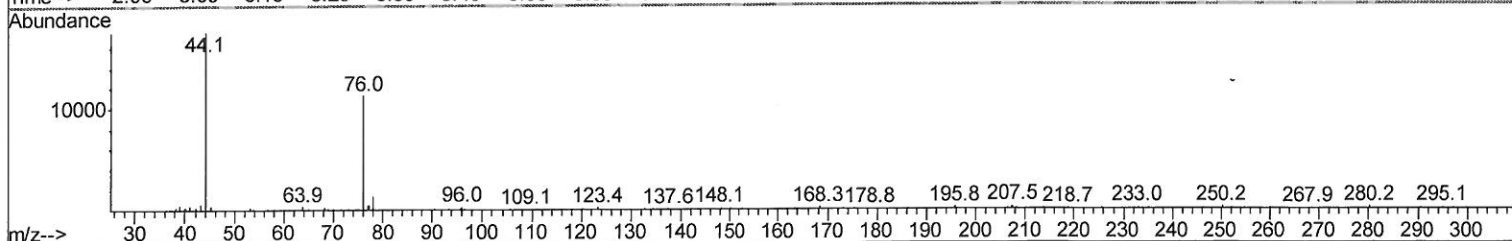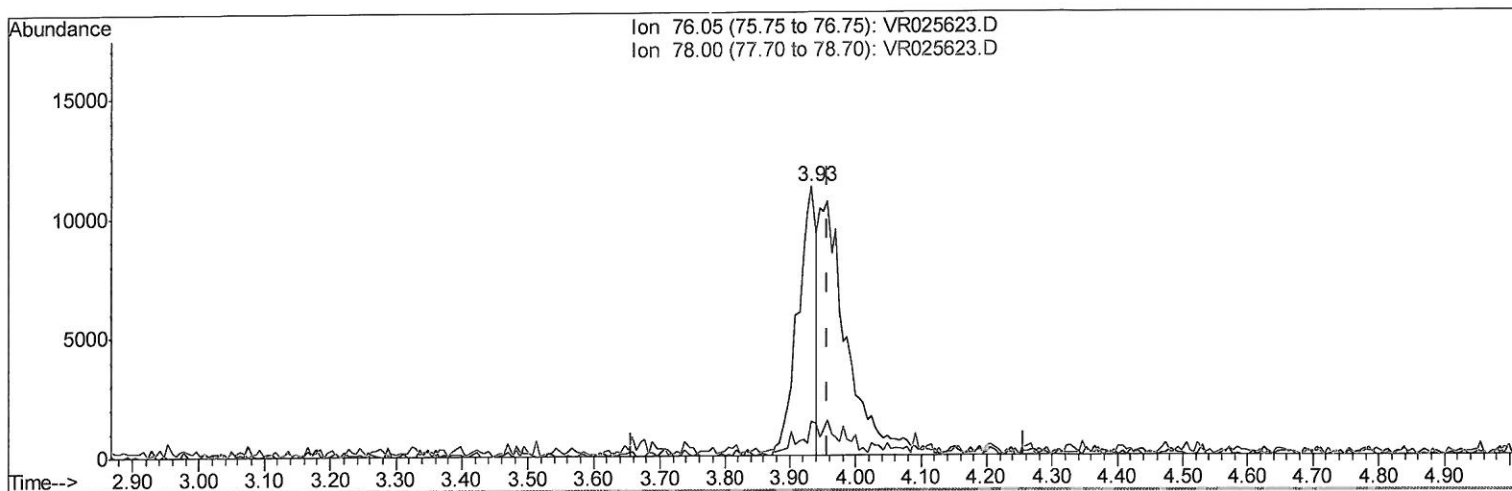

TIC: VR025623.D

(14) Carbon disulfide (T)

3.933min (-0.024) 0.22ug/L

response 21280

Ion	Exp%	Act%
76.05	100	100
78.00	10.10	12.68#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR082118\
Quantitation Report (Qedit)




Data File : VR025623.D
Acq On : 21 Aug 2018 12:04
Operator : SY/MD
Sample : VSTD0.581
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD0.581

Manual Integrations
APPROVED

MMDadoda
8/22/2018 10:49:49 AM

Quant Time: Aug 21 16:35:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR082118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 21 16:35:04 2018
Response via : Initial Calibration

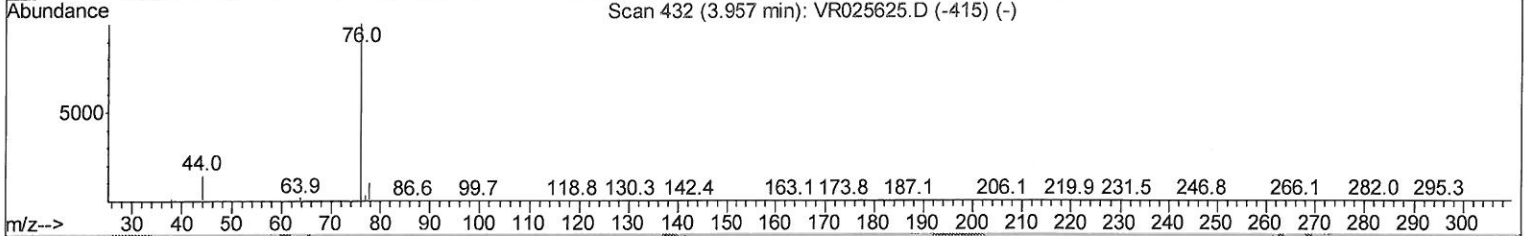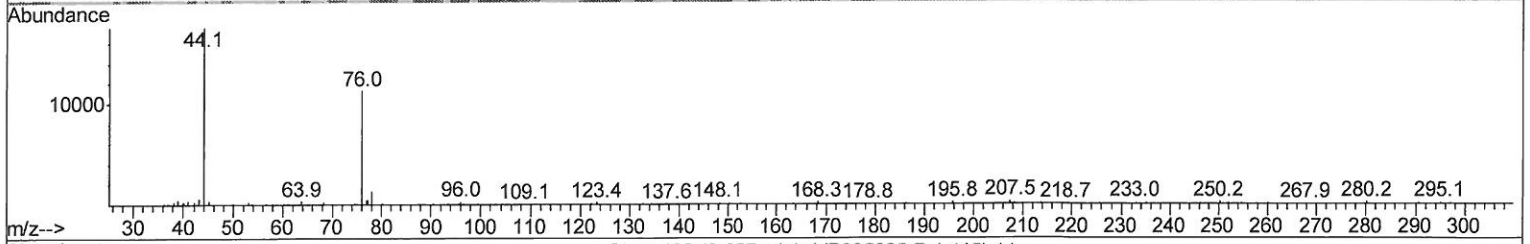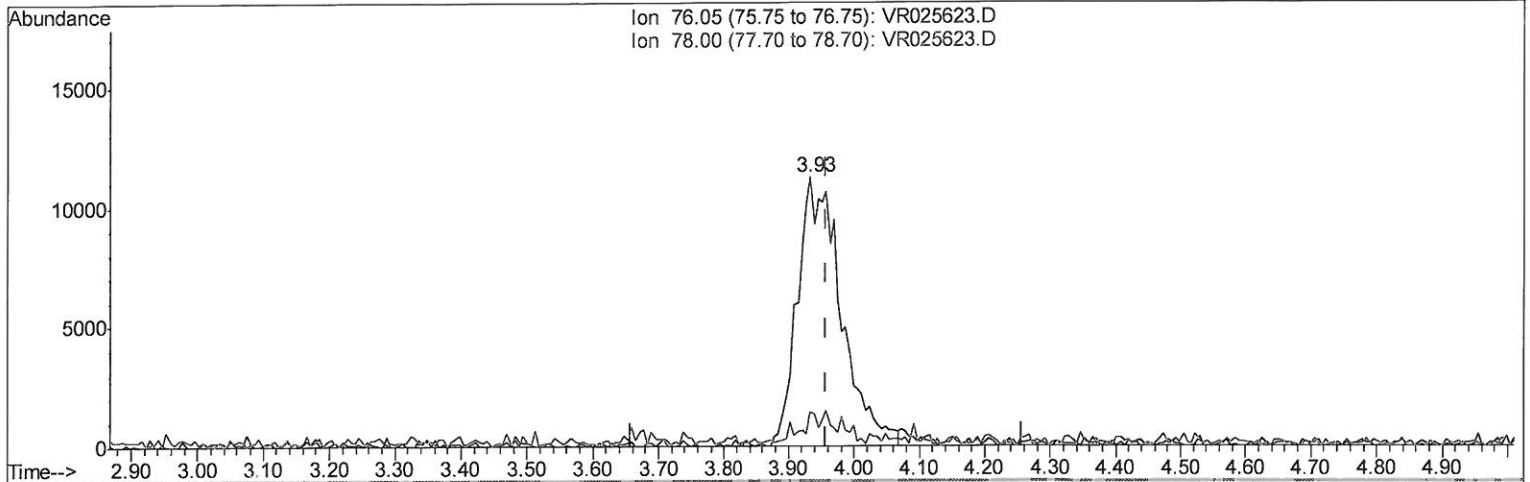

TIC: VR025623.D

(14) Carbon disulfide (T)

3.933min (-0.024) 0.54ug/L m

response 52198

Ion	Exp%	Act%
76.05	100	100
78.00	10.10	12.68#
0.00	0.00	0.00
0.00	0.00	0.00

208/22/1854




Data File : VR025623.D
Acq On : 21 Aug 2018 12:04
Operator : SY/MD
Sample : VSTD0.581
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD0.581

Manual Integrations
APPROVED

MMDadoda
8/22/2018 10:49:49 AM

Quant Time: Aug 21 16:35:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR082118WNA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 21 16:35:04 2018
Response via : Initial Calibration

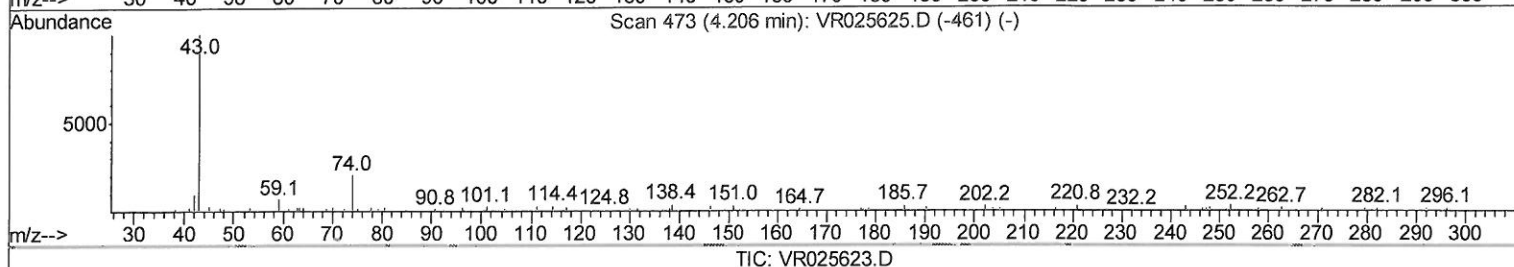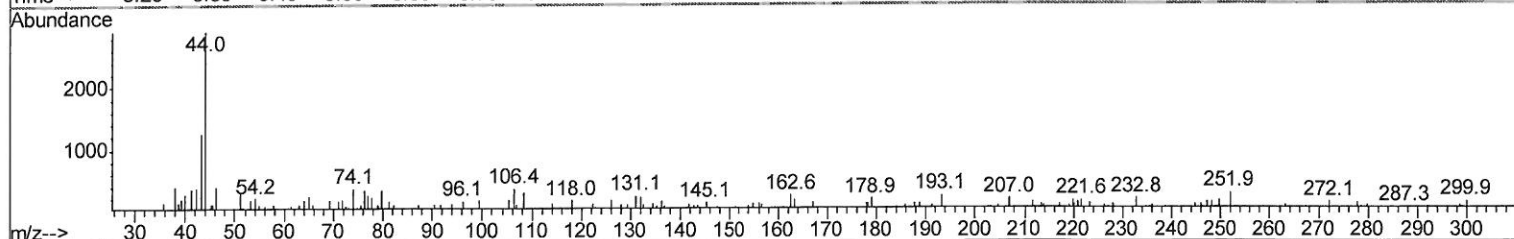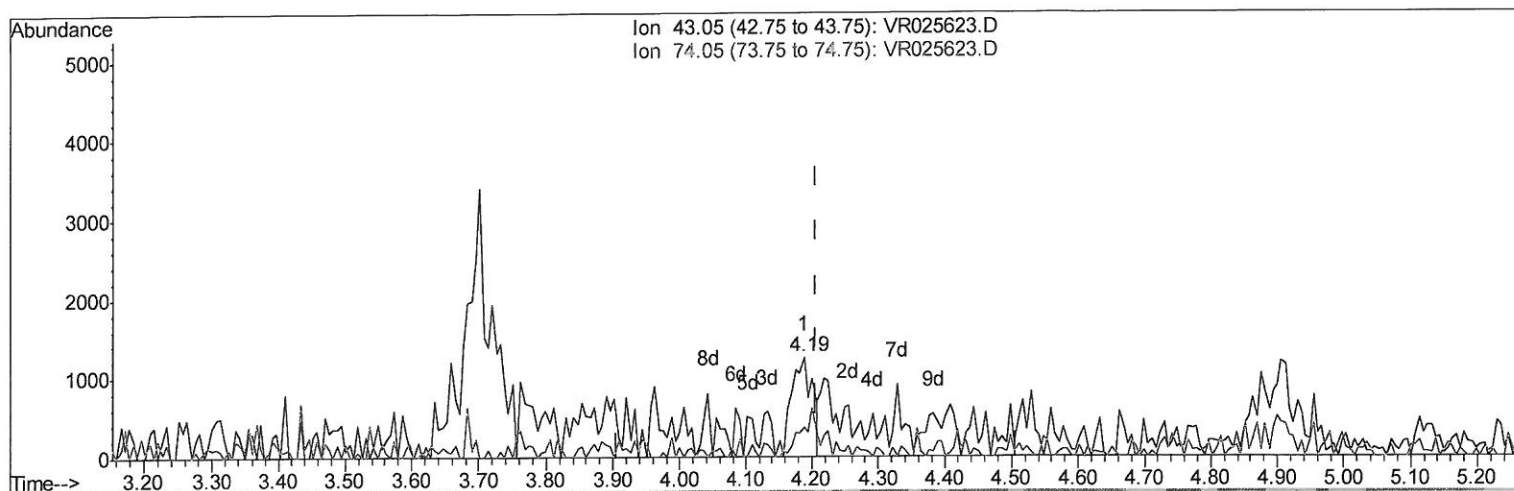

(15) Methyl Acetate (T)

4.188min (-0.018) 0.27ug/L

response 2651

Ion	Exp%	Act%
43.05	100	100
74.05	24.70	36.21#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR082118\
Quantitation Report (Qedit)




Data File : VR025623.D
Acq On : 21 Aug 2018 12:04
Operator : SY/MD
Sample : VSTD0.581
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD0.581

Manual Integrations
APPROVED

MMDadoda
8/22/2018 10:49:49 AM

Quant Time: Aug 21 16:35:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR082118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 21 16:35:04 2018
Response via : Initial Calibration

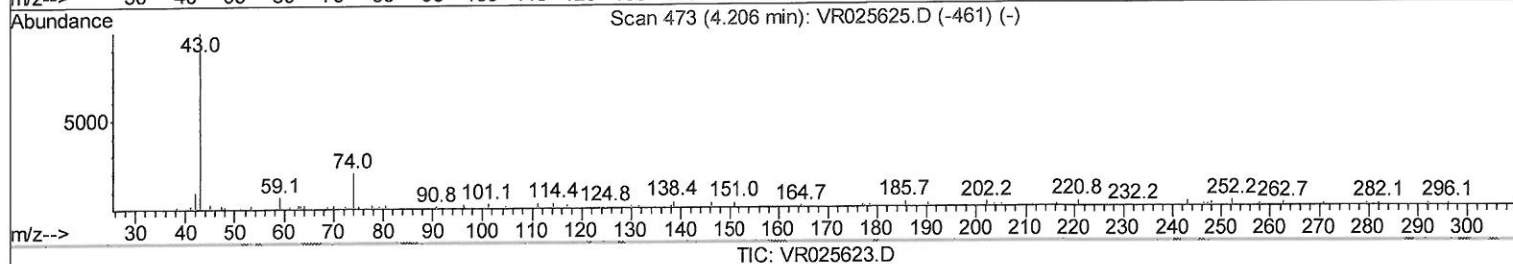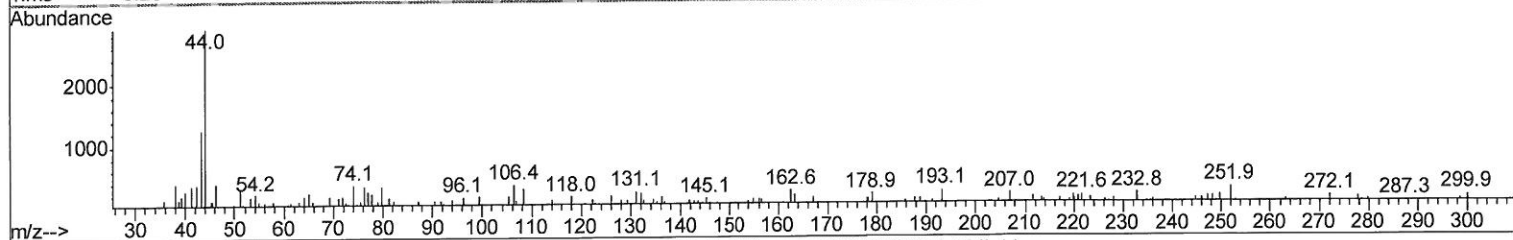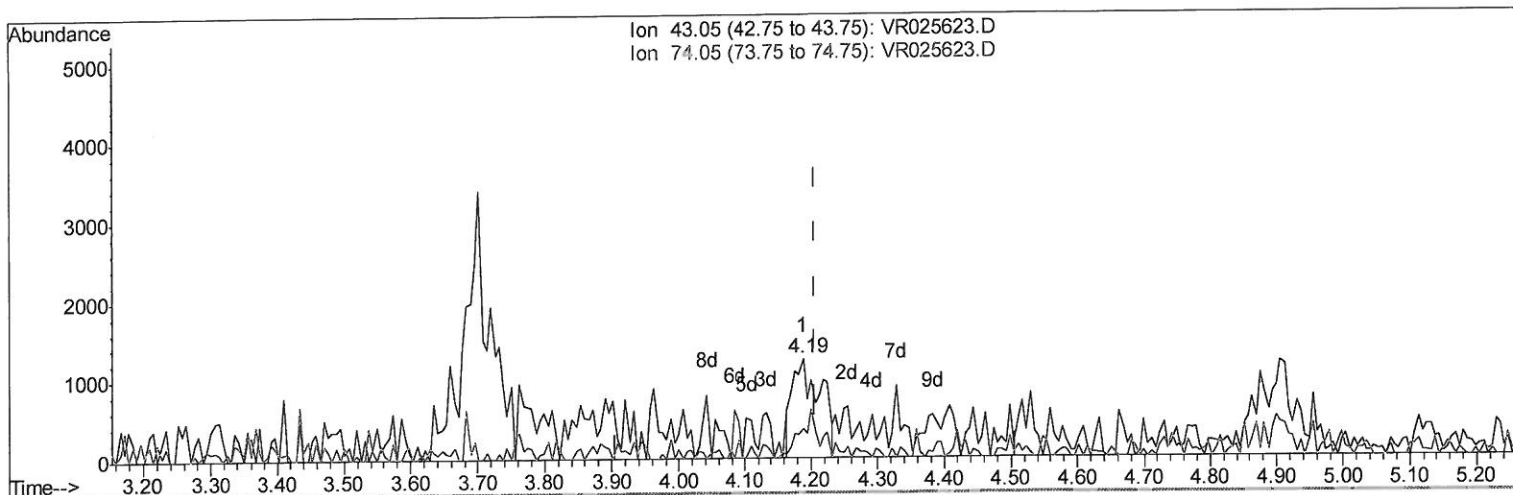

TIC: VR025623.D

(15) Methyl Acetate (T)

4.188min (-0.018) 0.36ug/L m

> 08/22/18 54

response 3593

Ion	Exp%	Act%
43.05	100	100
74.05	24.70	26.72
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR082118\
Quantitation Report (Qedit)




Data File : VR025623.D
Acq On : 21 Aug 2018 12:04
Operator : SY/MD
Sample : VSTD0.581
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD0.581

Manual Integrations
APPROVED

MMDadoda
8/22/2018 10:49:49 AM

Quant Time: Aug 21 16:35:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR082118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 21 16:35:04 2018
Response via : Initial Calibration

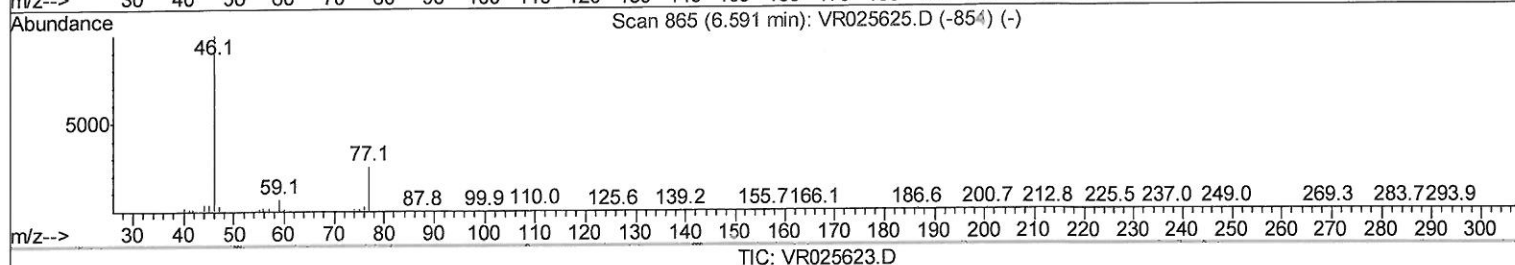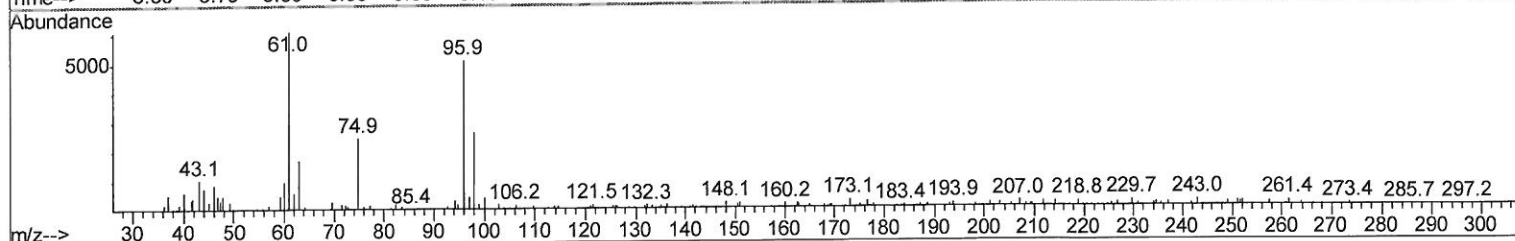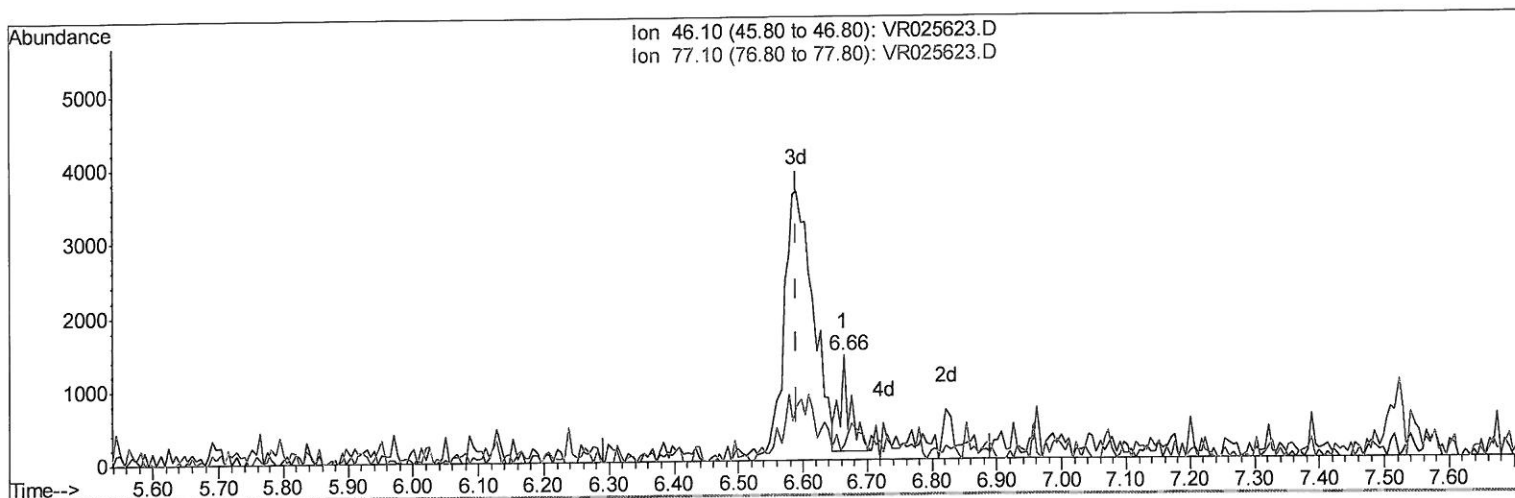

(20) 2-Butanone-d5 (S)

6.664min (+0.073) 0.41ug/L

response 1529

Ion	Exp%	Act%
46.10	100	100
77.10	25.00	32.44
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR082118\
Quantitation Report (Qedit)




Data File : VR025623.D
Acq On : 21 Aug 2018 12:04
Operator : SY/MD
Sample : VSTD0.581
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD0.581

Manual Integrations
APPROVED

MMDadoda
8/22/2018 10:49:49 AM

Quant Time: Aug 21 16:35:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR082118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 21 16:35:04 2018
Response via : Initial Calibration

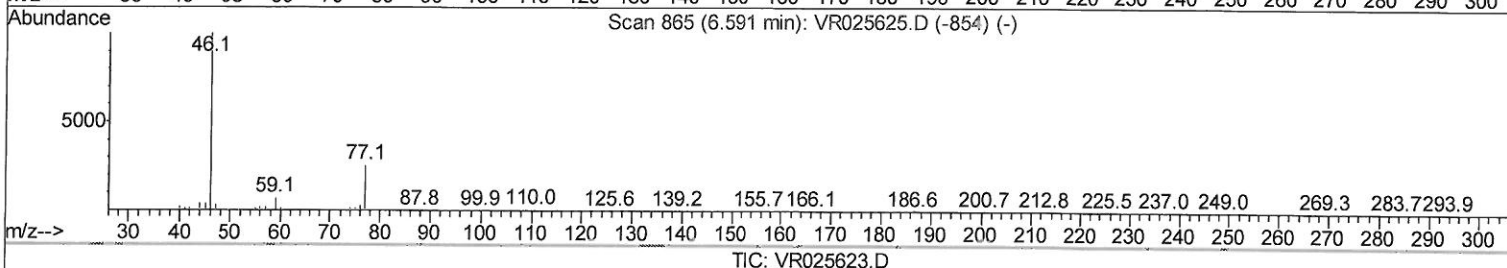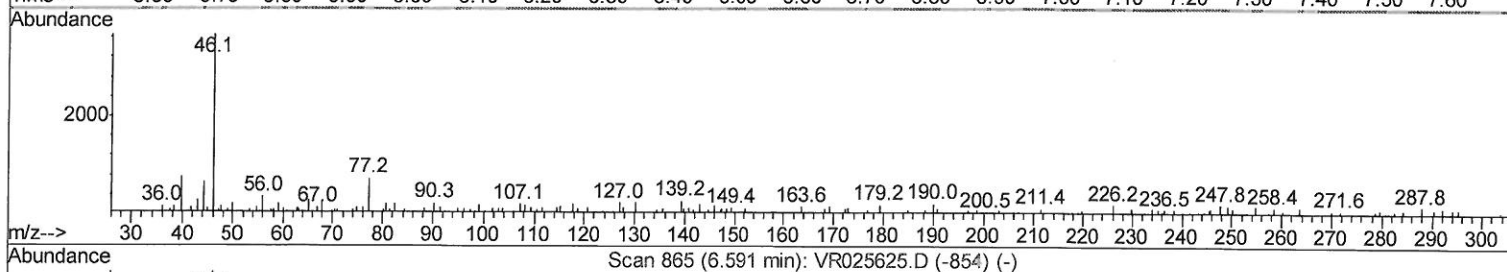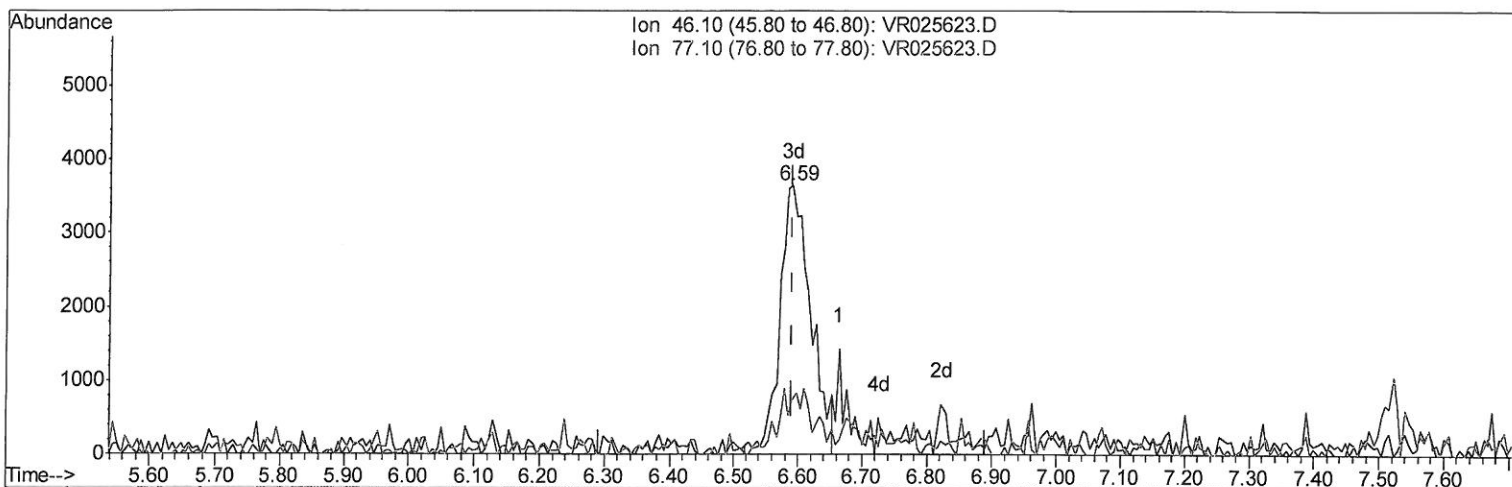

(20) 2-Butanone-d5 (S)

6.591min (+0.000) 3.25ug/L m

CS/22/18 SY

response 12040

Ion	Exp%	Act%
46.10	100	100
77.10	25.00	4.12#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR082118\
Quantitation Report (Qedit)




Data File : VR025623.D
Acq On : 21 Aug 2018 12:04
Operator : SY/MD
Sample : VSTD0.581
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD0.581

Manual Integrations
APPROVED

MMDadoda
8/22/2018 10:49:49 AM

Quant Time: Aug 21 16:35:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR082118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 21 16:35:04 2018
Response via : Initial Calibration

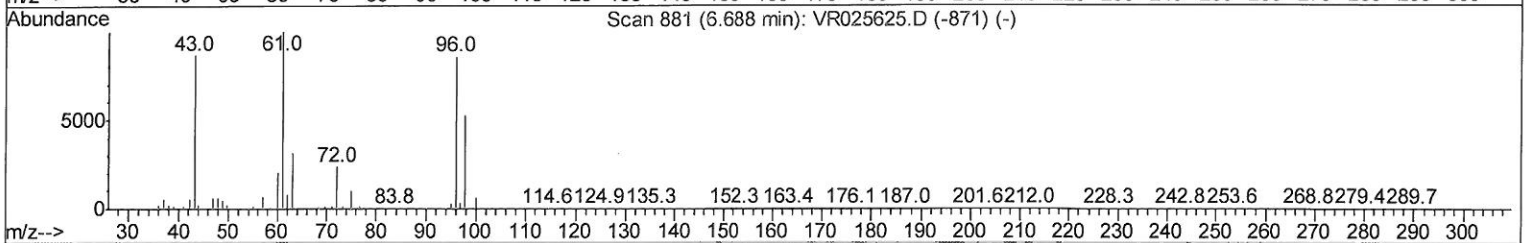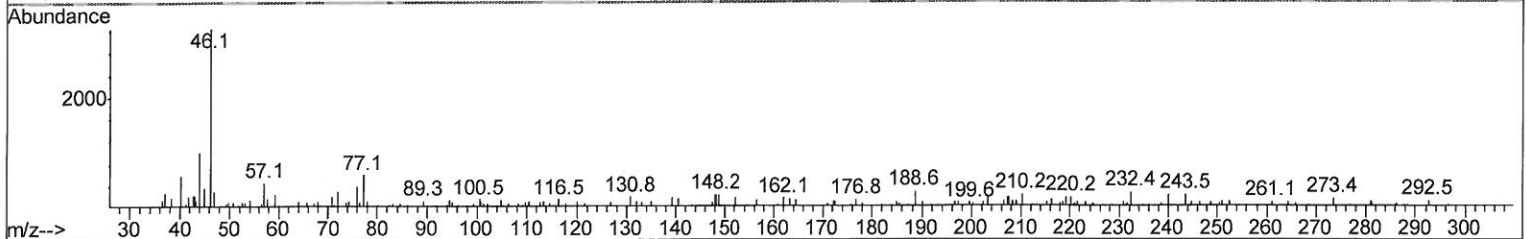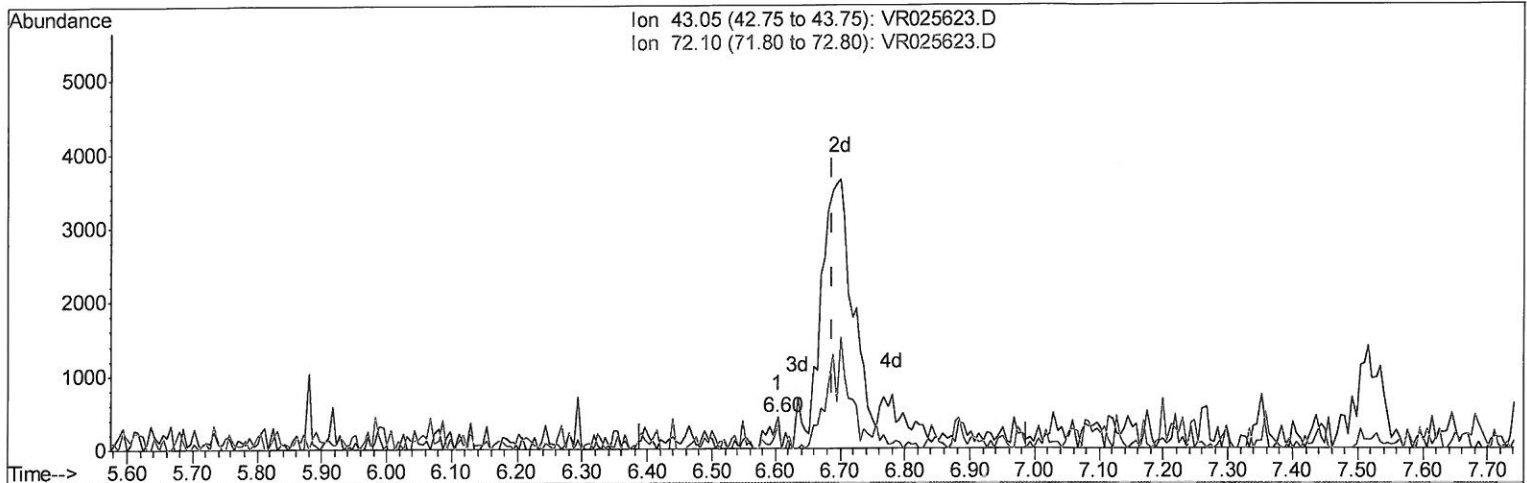

TIC: VR025623.D

(21) 2-Butanone (T)

6.603min (-0.085) 0.13ug/L

response 601

Ion	Exp%	Act%
43.05	100	100
72.10	28.60	40.10
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR082118\
Quantitation Report (Qedit)




Data File : VR025623.D
Acq On : 21 Aug 2018 12:04
Operator : SY/MD
Sample : VSTD0.581
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_R
Client Sampled :
VSTD0.581

Manual Integrations
APPROVED

MMDadoda
8/22/2018 10:49:49 AM

Quant Time: Aug 21 16:35:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR082118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 21 16:35:04 2018
Response via : Initial Calibration

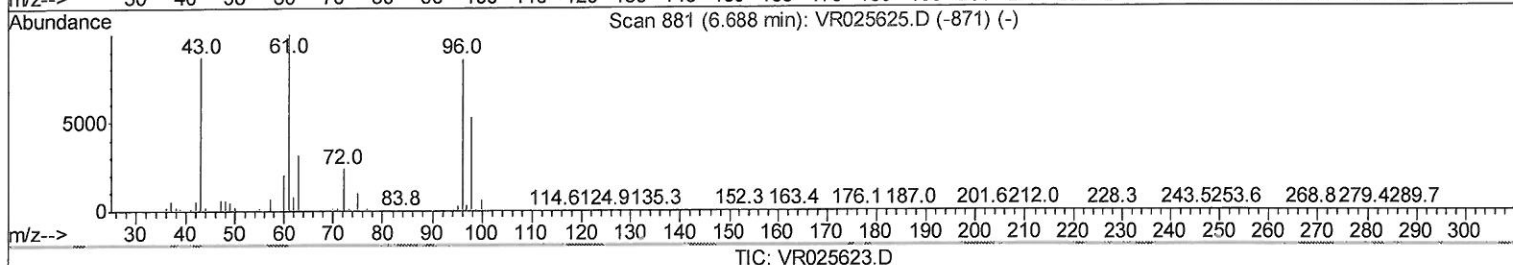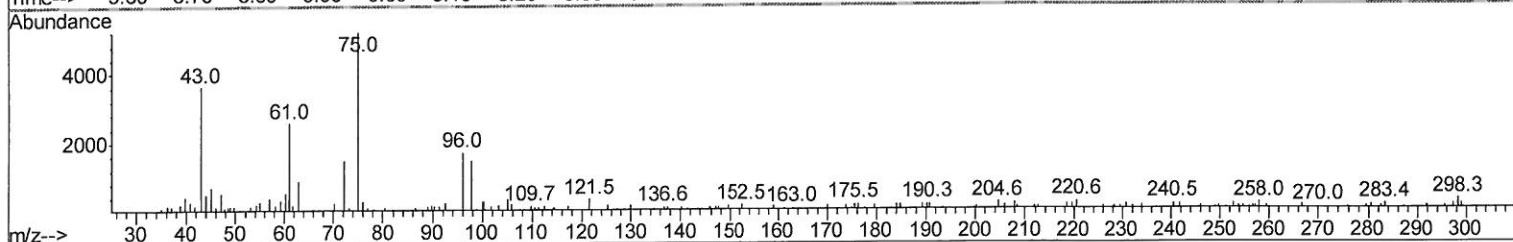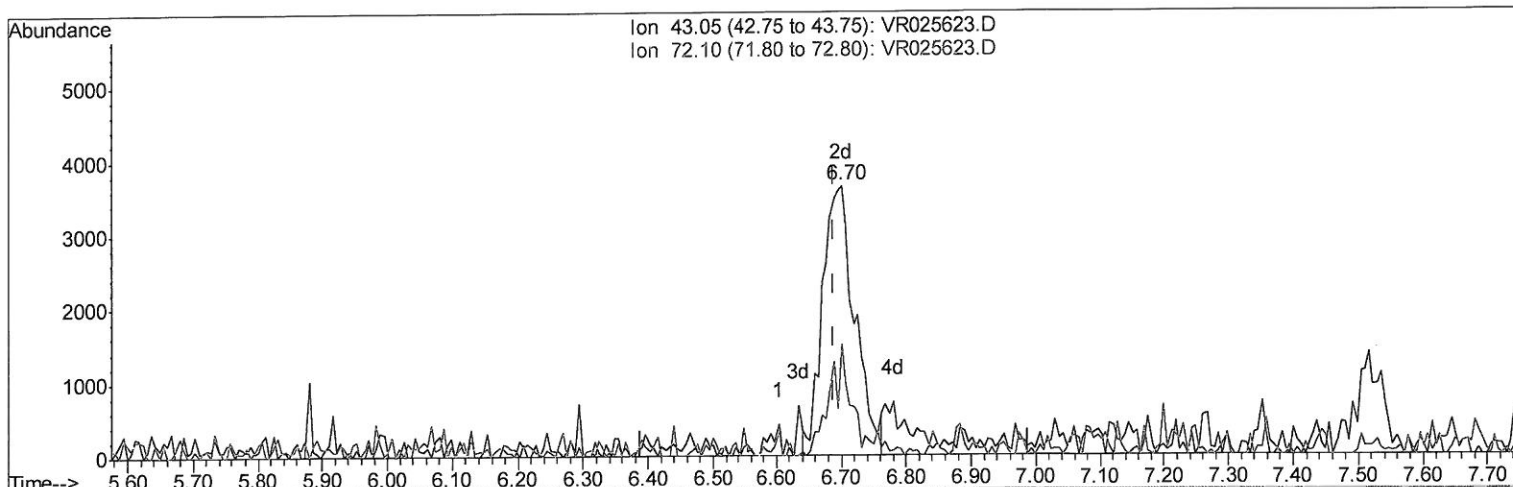

TIC: VR025623.D

(21) 2-Butanone (T)

6.701min (+0.012) 2.74ug/L m

> 08/22/18 sy

response 12630

Ion	Exp%	Act%
43.05	100	100
72.10	28.60	1.91#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR082118\
Quantitation Report (QT Reviewed)

Data File : VR025623.D
Acq On : 21 Aug 2018 12:04
Operator : SY/MD
Sample : VSTD0.581
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD0.581

Manual Integrations
APPROVED

MMDadoda
8/22/2018 10:49:49 AM

Quant Time: Aug 21 16:48:38 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR082118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 21 16:35:04 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	569267	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	472149	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	162600	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.16	65	17776	0.46	ug/L	0.00
7) Chloroethane-d5	2.61	69	16621	0.59	ug/L	0.00
11) 1,1-Dichloroethene-d2	3.62	63	44668	0.49	ug/L	0.00
20) 2-Butanone-d5	6.59	46	12040m	3.25	ug/L	0.00
24) Chloroform-d	7.21	84	30755	0.45	ug/L	0.00
26) 1,2-Dichloroethane-d4	7.91	65	11925	0.47	ug/L	0.02
32) Benzene-d6	7.86	84	72288	0.56	ug/L	0.00
36) 1,2-Dichloropropane-d6	8.90	67	18731	0.53	ug/L	0.00
41) Toluene-d8	9.97	98	61179	0.49	ug/L	0.00
43) trans-1,3-Dichloropropene-	10.24	79	3697	0.43	ug/L	0.00
46) 2-Hexanone-d5	10.59	63	9810	3.06	ug/L	0.00
57) 1,1,2,2-Tetrachloroethane-	12.37	84	8672	0.47	ug/L	0.00
64) 1,2-Dichlorobenzene-d4	13.51	152	12035	0.44	ug/L	0.00

Target Compounds

				Qvalue	
2) Dichlorodifluoromethane	1.83	85	14491m	0.436	ug/L
3) Chloromethane	2.00	50	22411	0.447	ug/L
5) Vinyl chloride	2.16	62	20970	0.465	ug/L
6) Bromomethane	2.52	94	15387	0.706	ug/L
8) Chloroethane	2.64	64	12142	0.510	ug/L
9) Trichlorofluoromethane	2.99	101	31577m	0.482	ug/L
10) 1,1,2-Trichloro-1,2,2-trif	3.67	101	19617	0.463	ug/L
12) 1,1-Dichloroethene	3.63	96	23282	0.497	ug/L
13) Acetone	3.70	43	8679m	2.285	ug/L
14) Carbon disulfide	3.93	76	52198m	0.540	ug/L
15) Methyl Acetate	4.19	43	3593m	0.360	ug/L
16) Methylene chloride	4.41	84	20379	0.470	ug/L
17) Methyl tert-butyl Ether	4.90	73	17432	0.354	ug/L #
18) trans-1,2-Dichloroethene	4.88	96	21924	0.496	ug/L #
19) 1,1-Dichloroethane	5.70	63	33420	0.531	ug/L #
21) 2-Butanone	6.70	43	12630m	2.735	ug/L
22) cis-1,2-Dichloroethene	6.67	96	15368	0.386	ug/L #
23) Bromochloromethane	7.06	128	5749	0.380	ug/L #
25) Chloroform	7.24	83	28429	0.431	ug/L
27) 1,2-Dichloroethane	8.00	62	9014	0.339	ug/L #
29) 1,1,1-Trichloroethane	7.42	97	21554	0.538	ug/L
30) Cyclohexane	7.52	56	24141	0.612	ug/L
31) Carbon tetrachloride	7.64	117	18872	0.448	ug/L
33) Benzene	7.91	78	73299	0.498	ug/L
34) Trichloroethene	8.70	95	18276	0.523	ug/L
35) Methylcyclohexane	3.96	83	24801	0.523	ug/L
37) 1,2-Dichloropropane	8.99	63	17705	0.526	ug/L #
38) Bromodichloromethane	9.28	83	15625	0.466	ug/L #
39) cis-1,3-Dichloropropene	9.72	75	14739	0.444	ug/L
40) 4-Methyl-2-pentanone	9.86	43	28959	2.861	ug/L

08/22/18 SY

08/22/18 SY

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR082118\
Quantitation Report (QT Reviewed)

Data File : VR025623.D
Acq On : 21 Aug 2018 12:04
Operator : SY/MD
Sample : VSTD0.581
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD0.581

Manual Integrations
APPROVED

MMDadoda
8/22/2018 10:49:49 AM

Quant Time: Aug 21 16:48:38 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR082118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 21 16:35:04 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
42) Toluene	10.03	91	64985	0.409	ug/L	93
44) trans-1,3-Dichloropropene	10.27	75	9653	0.392	ug/L	93
45) 1,1,2-Trichloroethane	10.45	97	8185	0.459	ug/L #	86
47) Tetrachloroethene	10.51	164	14680	0.476	ug/L	80
48) 2-Hexanone	10.63	43	18608	2.622	ug/L #	97
49) Dibromochloromethane	10.78	129	6994	0.331	ug/L	82
50) 1,2-Dibromoethane	10.89	107	5514	0.362	ug/L #	92
51) Chlorobenzene	11.31	112	50016	0.494	ug/L	98
52) Ethylbenzene	11.39	91	70109	0.438	ug/L	95
53) m,p-Xylene	11.51	106	27959	0.441	ug/L	93
54) o-Xylene	11.83	106	21225	0.359	ug/L	98
55) Styrene	11.85	104	32881	0.337	ug/L	94
56) Isopropylbenzene	12.13	105	54415	0.383	ug/L	96
58) 1,1,2,2-Tetrachloroethane	12.38	83	6826	0.381	ug/L	99
59) 1,2,3-Trichloropropane	12.44	75	5202	0.466	ug/L #	70
61) Bromoform	12.01	173	3032	0.400	ug/L #	97
62) 1,3-Dichlorobenzene	13.16	146	22133	0.472	ug/L	90
63) 1,4-Dichlorobenzene	13.25	146	28078	0.496	ug/L	90
65) 1,2-Dichlorobenzene	13.53	146	20507	0.459	ug/L #	81
66) 1,2-Dibromo-3-chloropropan	14.15	75	446	0.333	ug/L	87
67) 1,3,5-Trichlorobenzene	14.29	180	11230	0.356	ug/L #	85
68) 1,2,4-trichlorobenzene	14.79	180	7542	0.388	ug/L	99
69) Naphthalene	15.00	128	7640	0.336	ug/L #	89
70) 1,2,3-Trichlorobenzene	15.18	180	5810	0.352	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed