
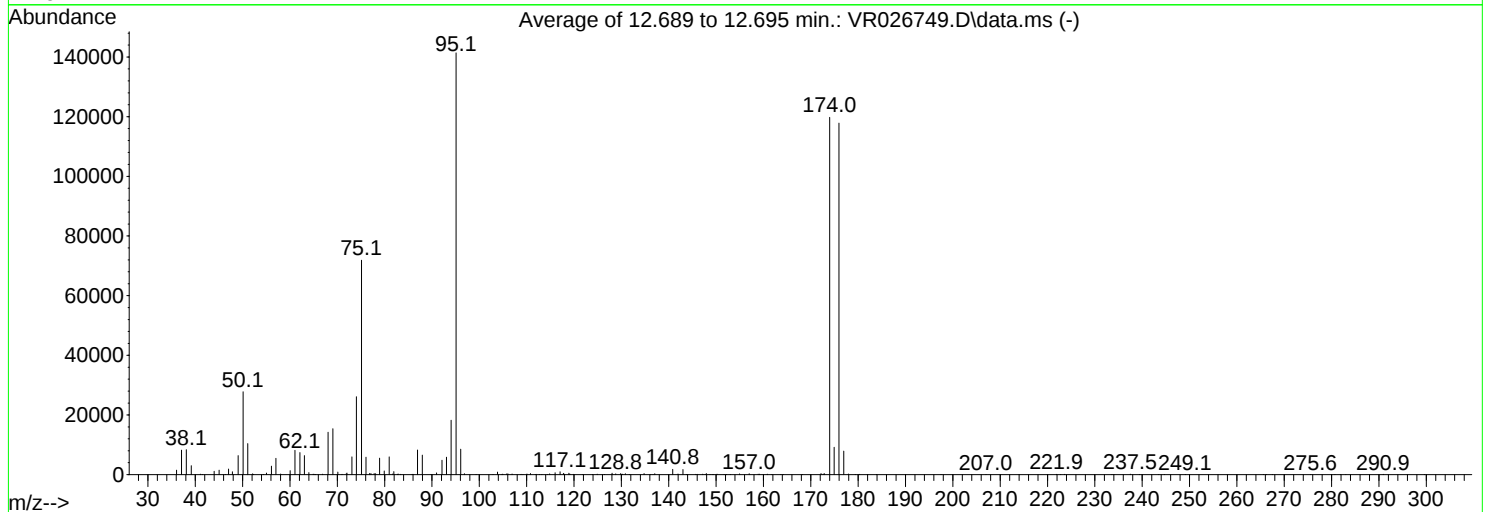


Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR082125\
Data File : VR026749.D
Acq On : 21 Aug 2025 8:00
Operator : SY/MD
Sample : BFB
Misc : 5mL/MSVOA_R/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_R\methods\82R082025W.M
Title : SW846 8260
Last Update : Thu Aug 21 08:59:04 2025

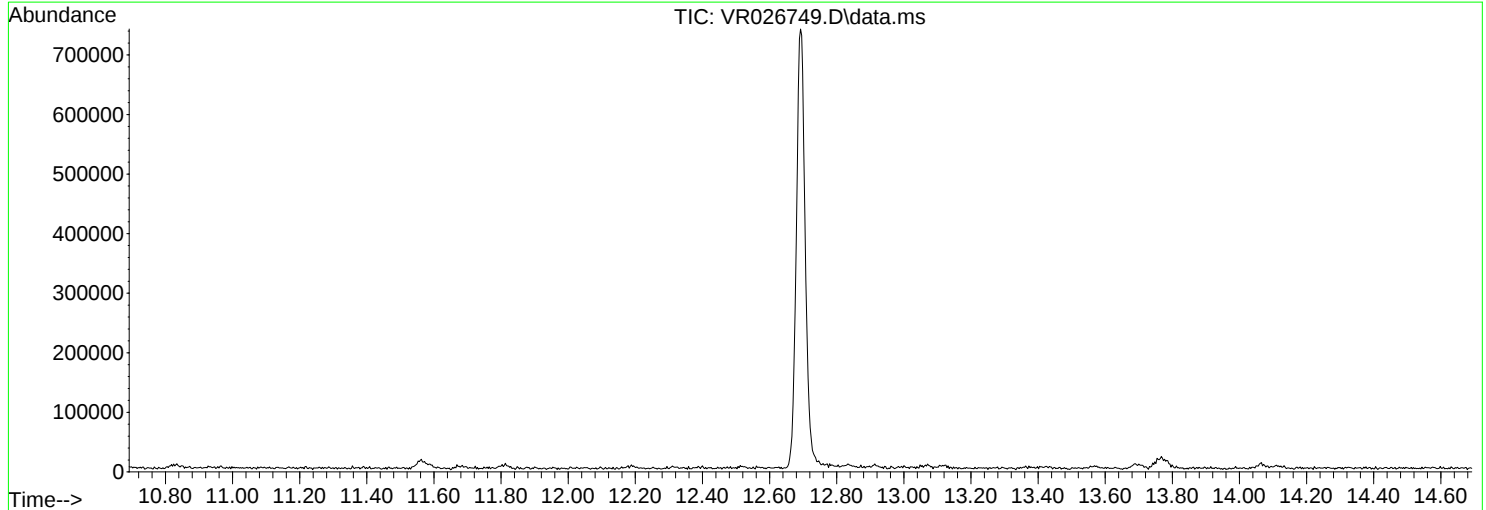

AutoFind: Scans 3773, 3774, 3775; Background Corrected with Scan 3757

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	27787	PASS
75	95	30	60	50.8	71875	PASS
95	95	100	100	100.0	141397	PASS
96	95	5	9	6.0	8552	PASS
173	174	0.00	2	0.3	356	PASS
174	95	50	100	84.7	119781	PASS
175	174	5	9	7.6	9159	PASS
176	174	95	101	98.4	117851	PASS
177	176	5	9	6.7	7897	PASS