

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR082418\
 Data File : VR025633.D
 Acq On : 24 Aug 2018 14:10
 Operator : SY/MD
 Sample : J4601-01
 Misc : 25mL/MSVOA_R/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 C0SX6

Quant Time: Aug 25 00:00:16 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR082118WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 24 23:05:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	446213	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	365069	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	109550	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	146487	5.04	ug/L	-0.02
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.80%
7) Chloroethane-d5	2.62	69	127634	5.09	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.80%
11) 1,1-Dichloroethene-d2	3.63	63	241579	3.37	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.40%
20) 2-Butanone-d5	6.59	46	136128	61.51	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	123.02%
24) Chloroform-d	7.20	84	237866	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.20%
26) 1,2-Dichloroethane-d4	7.89	65	82095	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.60%
32) Benzene-d6	7.86	84	567448	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.00%
36) 1,2-Dichloropropane-d6	8.90	67	156963	5.16	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.20%
41) Toluene-d8	9.97	98	506198	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.80%
43) trans-1,3-Dichloropropene-	10.24	79	30785	4.29	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.80%
46) 2-Hexanone-d5	10.59	63	131843	56.12	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	112.24%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	60622	4.32	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.40%
64) 1,2-Dichlorobenzene-d4	13.51	152	106828	6.10	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	122.00%#


Target Compounds					Qvalue
13) Acetone	3.70	43	6367	4.618 ug/L	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_R\DATA\VR082418\
Data File : VR025633.D
Acq On : 24 Aug 2018 14:10
Operator : SY/MD
Sample : J4601-01
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
C0SX6

Quant Time: Aug 25 00:00:16 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR082118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 24 23:05:03 2018
Response via : Initial Calibration

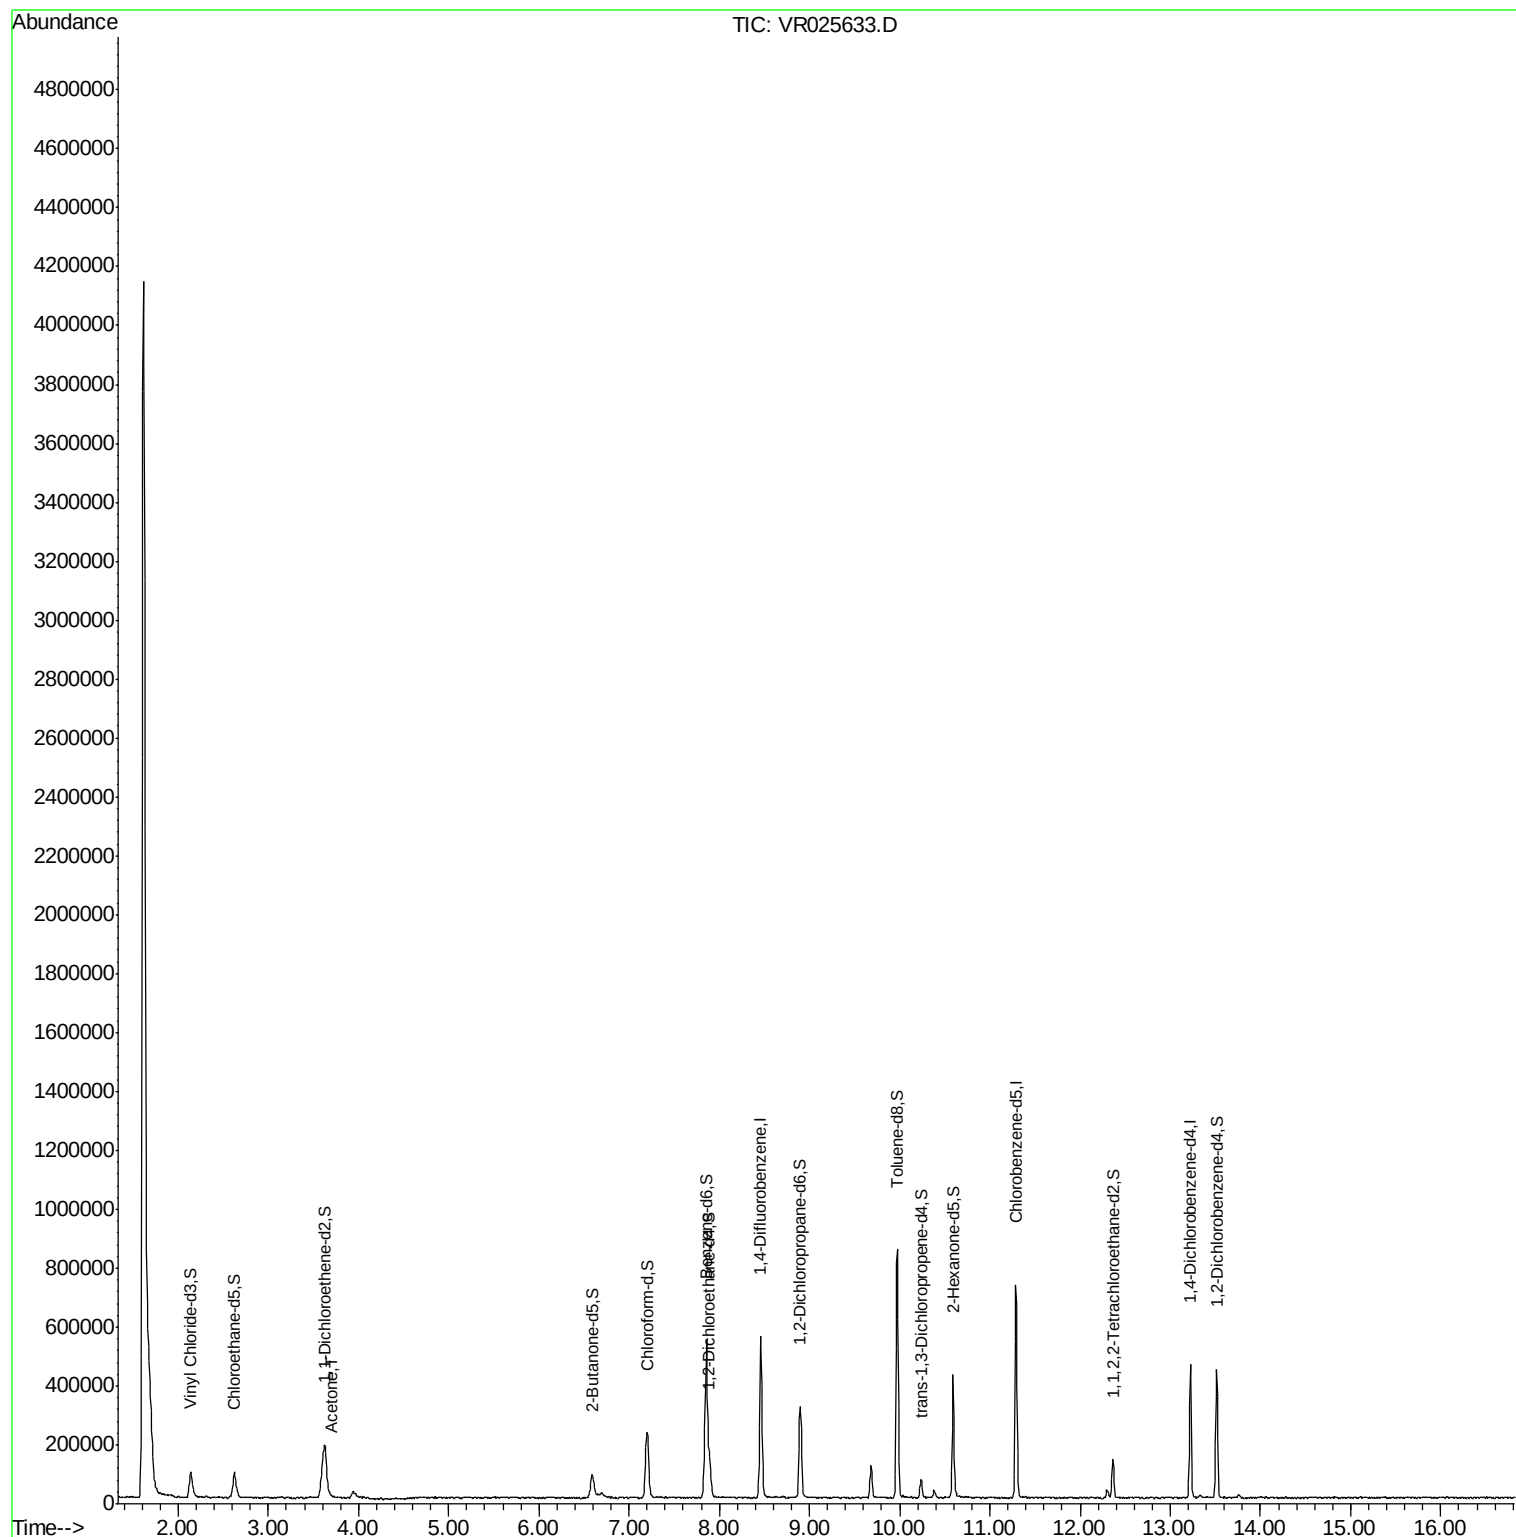

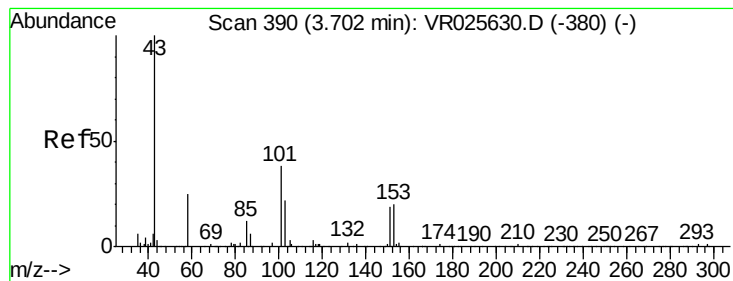

#13

Acetone

Concen: 4.618 ug/L

RT: 3.70 min Scan# 390

Delta R.T. 0.00 min

Lab File: VR025633.D

Acq: 24 Aug 2018 14:10

Instrument :
MSVOA_R
ClientSampleId :
C0SX6

Tgt Ion: 43 Resp: 6367

Ion Ratio Lower Upper

43 100

58 16.9 0.0 63.4

