
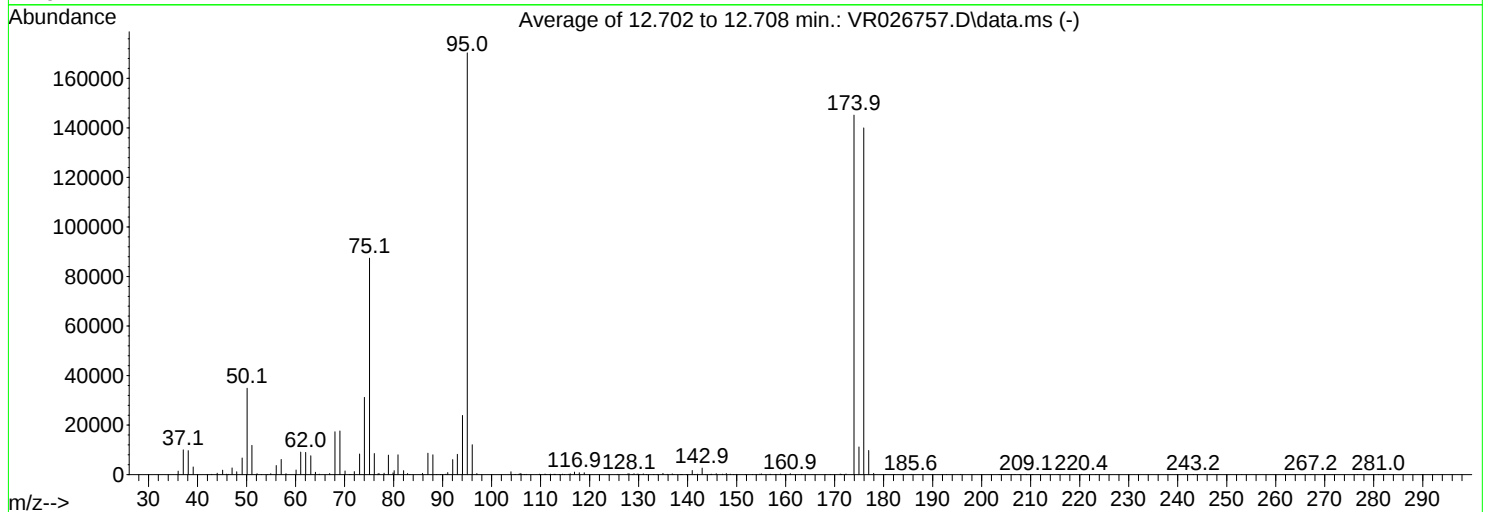


Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR082525\
Data File : VR026757.D
Acq On : 25 Aug 2025 11:18
Operator : SY/MD
Sample : BFB
Misc : 5mL/MSVOA_R/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_R\methods\82R082025W.M
Title : SW846 8260
Last Update : Thu Aug 21 08:59:04 2025

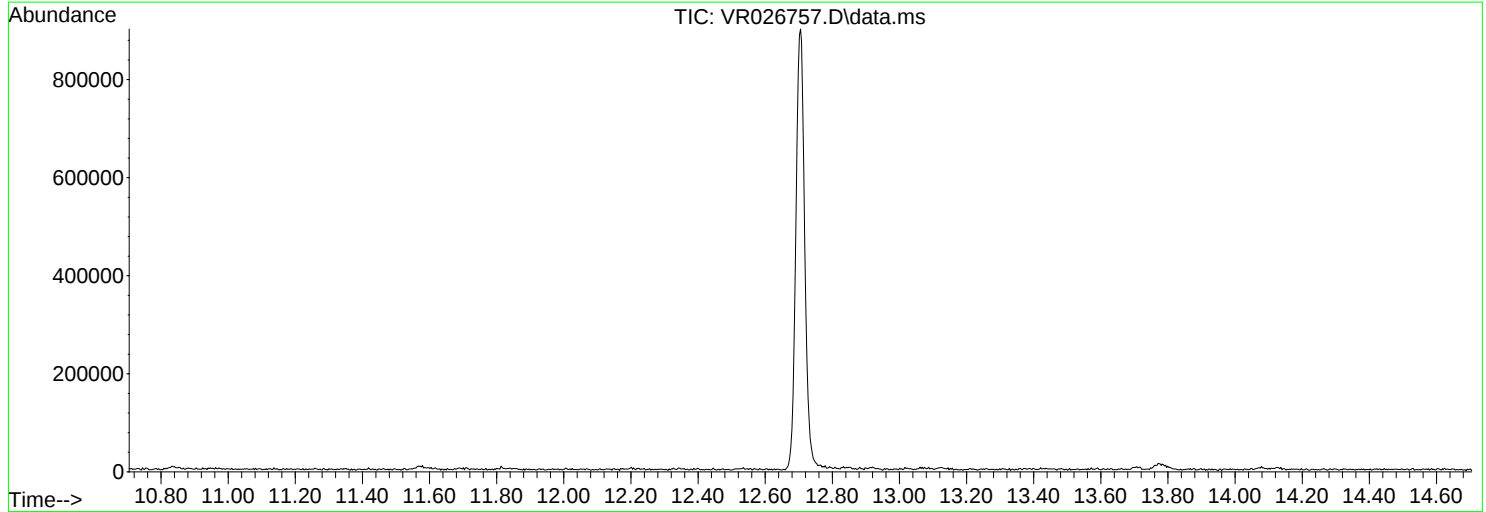

AutoFind: Scans 3777, 3778, 3779; Background Corrected with Scan 3762

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.5	34907	PASS
75	95	30	60	51.3	87435	PASS
95	95	100	100	100.0	170304	PASS
96	95	5	9	7.1	12094	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	85.2	145173	PASS
175	174	5	9	7.7	11159	PASS
176	174	95	101	96.4	139968	PASS
177	176	5	9	7.0	9756	PASS