

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR091318\
 Data File : VR025713.D
 Acq On : 13 Sep 2018 14:00
 Operator : SY/MD
 Sample : J4633-02
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 DB3J6

Quant Time: Sep 14 07:16:01 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR090718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 14 06:42:34 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	695877	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	589775	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	168062	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.15	65	123214	4.07	ug/L	-0.01
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.40%
7) Chloroethane-d5	2.63	69	106796	4.31	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.20%
11) 1,1-Dichloroethene-d2	3.63	63	251044	3.03	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.60%
20) 2-Butanone-d5	6.59	46	159060	52.08	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.16%
24) Chloroform-d	7.20	84	291629	4.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.20%
26) 1,2-Dichloroethane-d4	7.90	65	101907	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.80%
32) Benzene-d6	7.85	84	666867	4.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.60%
36) 1,2-Dichloropropane-d6	8.90	67	190260	4.43	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.60%
41) Toluene-d8	9.97	98	623051	4.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.80%
43) trans-1,3-Dichloropropene-	10.24	79	36499	3.44	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.80%
46) 2-Hexanone-d5	10.59	63	154976	48.88	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.76%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	79242	4.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.40%
64) 1,2-Dichlorobenzene-d4	13.52	152	140201	5.89	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.80%


Target Compounds					Ovalue
13) Acetone	3.70	43	17928	8.71 ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR091318\
Data File : VR025713.D
Acq On : 13 Sep 2018 14:00
Operator : SY/MD
Sample : J4633-02
Misc : 25mL/MSVOA R/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
DB3J6

Quant Time: Sep 14 07:16:01 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR090718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 14 06:42:34 2018
Response via : Initial Calibration

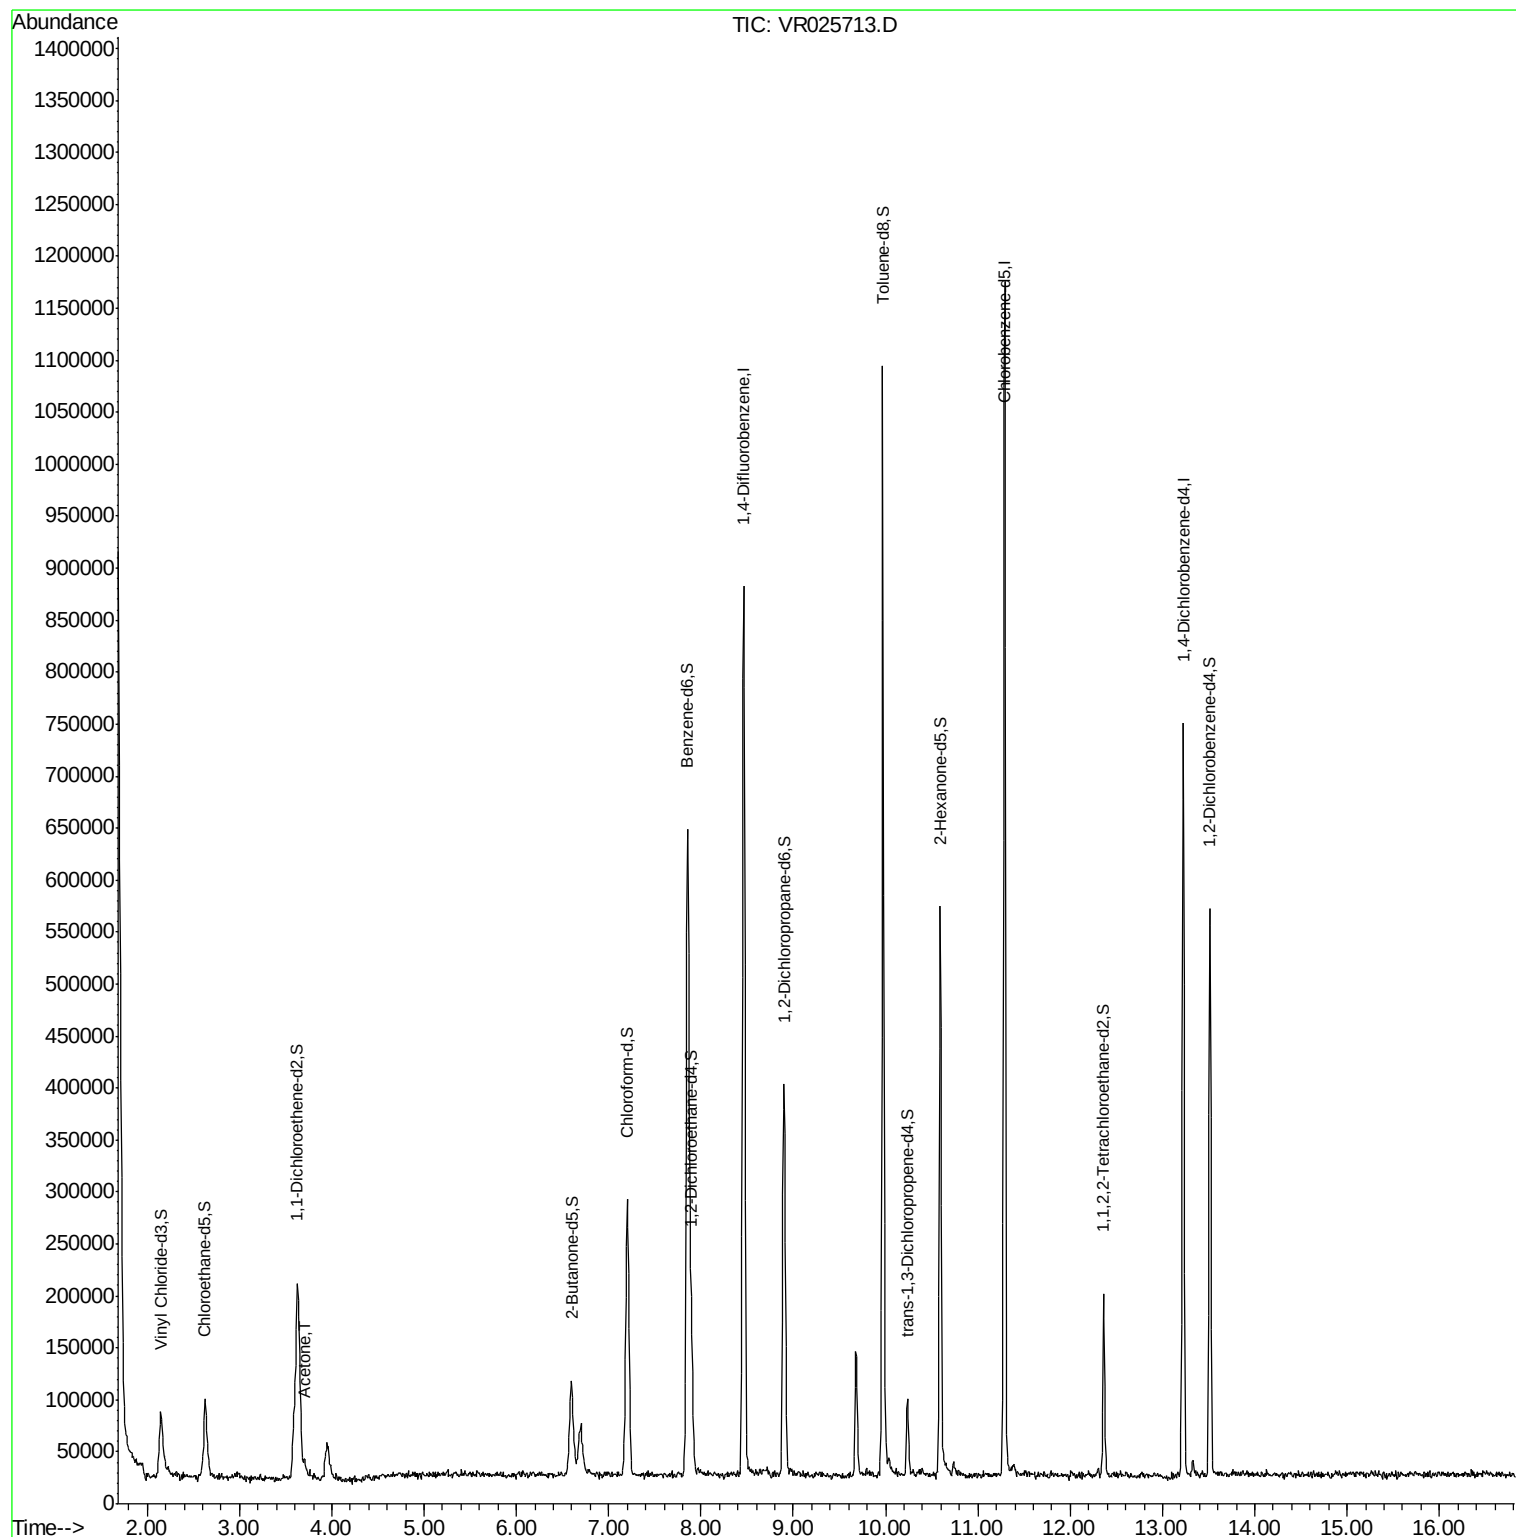

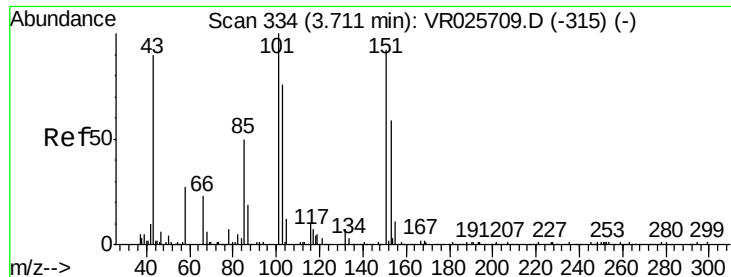

#13

Acetone

Concen: 8.71 ug/L

RT: 3.70 min Scan# 333

Delta R.T. -0.01 min

Lab File: VR025713.D

Acq: 13 Sep 2018 14:00

Instrument :
MSVOA_R
ClientSampleId :
DB3J6

Tot Ion: 43 Resp: 17928

Ion Ratio Lower Upper

43 100

58 33.7 0.0 53.6

