




Data File : VR026636.D
Acq On : 13 Sep 2019 17:20
Operator : SY/MD
Sample : MDL02
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL02

Manual Integrations
APPROVED

MMDadoda
9/16/2019 12:45:01 AM

Quant Time: Sep 14 06:52:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 06:49:16 2019
Response via : Initial Calibration

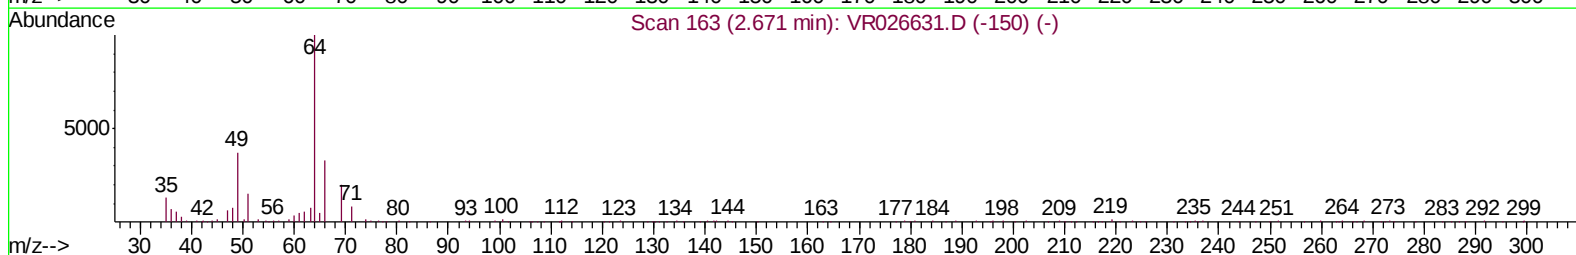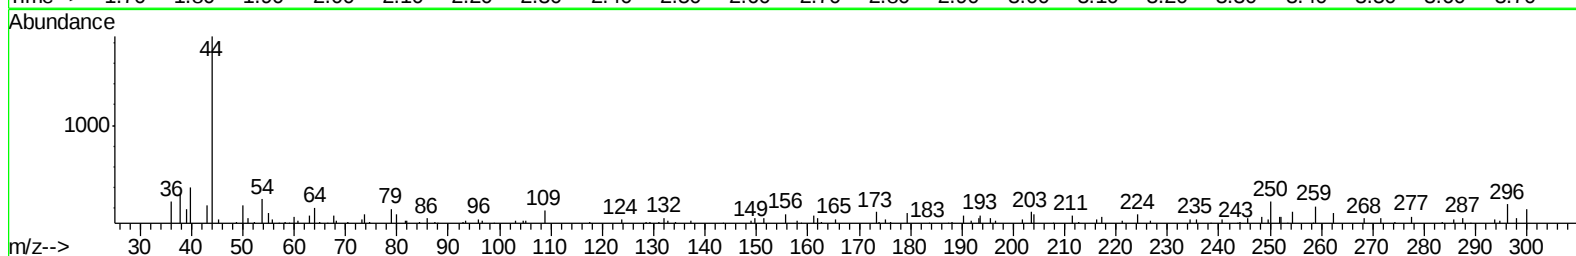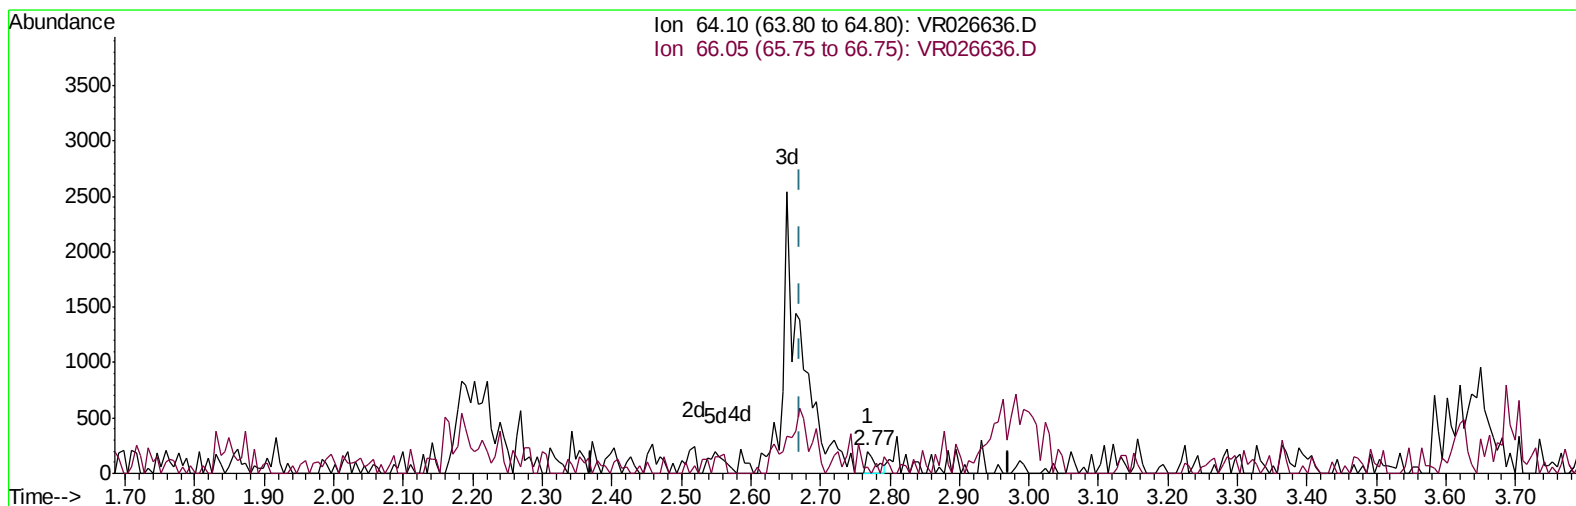

TIC: VR026636.D

(8) Chloroethane (T)

2.768min (+0.097) 0.02ug/L

response 207

Ion	Exp%	Act%
64.10	100	100
66.05	31.80	26.37
0.00	0.00	0.00
0.00	0.00	0.00




Data File : VR026636.D
Acq On : 13 Sep 2019 17:20
Operator : SY/MD
Sample : MDL02
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL02

Manual Integrations
APPROVED

MMDadoda
9/16/2019 12:45:01 AM

Quant Time: Sep 14 06:52:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 06:49:16 2019
Response via : Initial Calibration

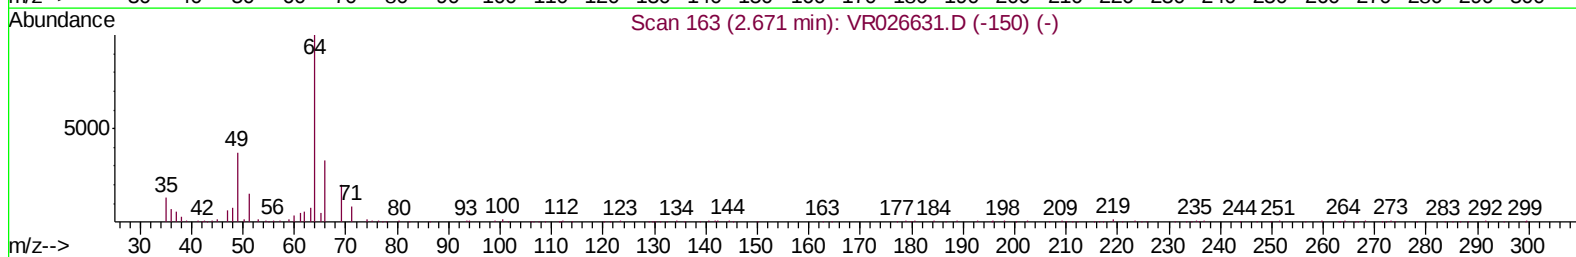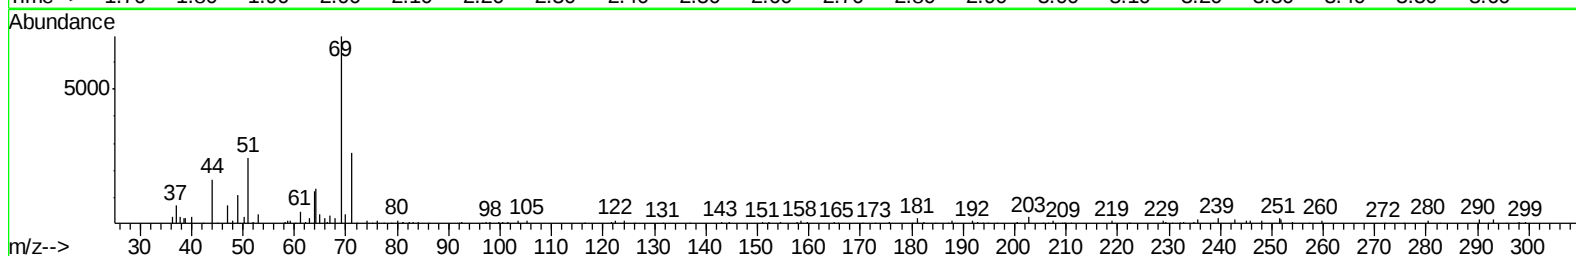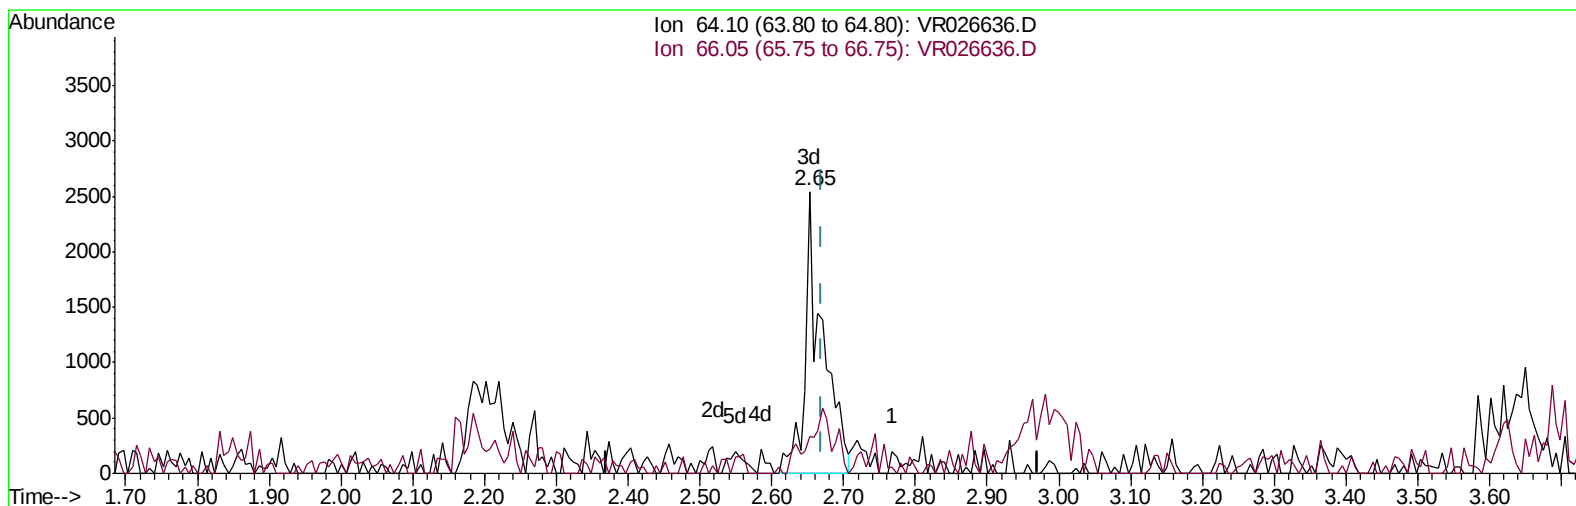

TIC: VR026636.D

(8) Chloroethane (T)

2.652min (-0.018) 0.40ug/L m

response 4327

Ion	Exp%	Act%
64.10	100	100
66.05	31.80	17.29#
0.00	0.00	0.00
0.00	0.00	0.00




Data File : VR026636.D
Acq On : 13 Sep 2019 17:20
Operator : SY/MD
Sample : MDL02
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL02

Manual Integrations
APPROVED

MMDadoda
9/16/2019 12:45:01 AM

Quant Time: Sep 14 06:52:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 06:49:16 2019
Response via : Initial Calibration

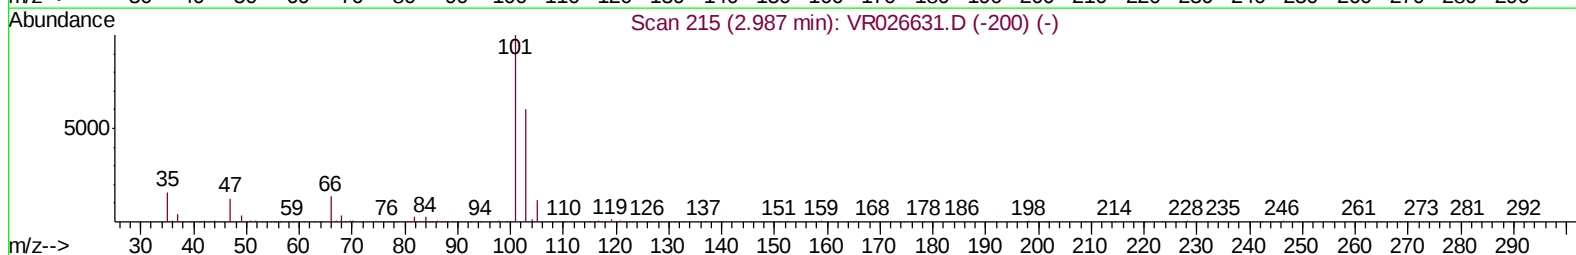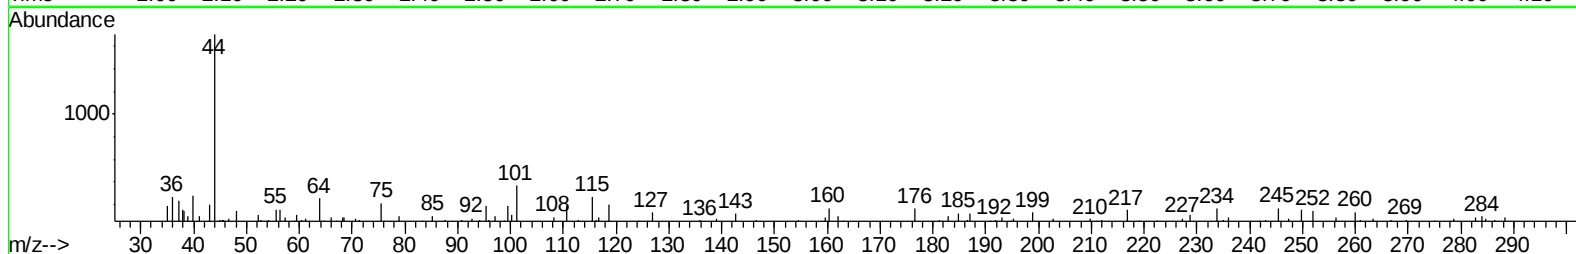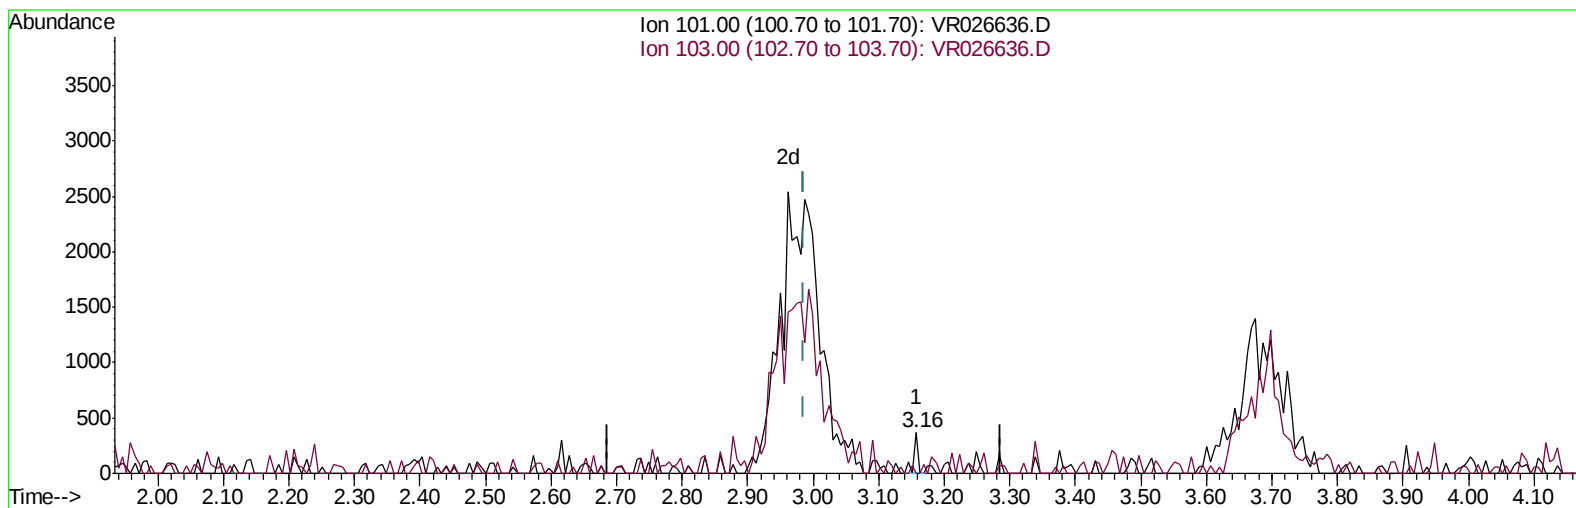

TIC: VR026636.D

(9) Trichlorofluoromethane (T)

3.157min (+0.170) 0.01ug/L

response 171

Ion	Exp%	Act%
101.00	100	100
103.00	63.60	69.59
0.00	0.00	0.00
0.00	0.00	0.00




Data File : VR026636.D
Acq On : 13 Sep 2019 17:20
Operator : SY/MD
Sample : MDL02
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL02

Manual Integrations
APPROVED

MMDadoda
9/16/2019 12:45:01 AM

Quant Time: Sep 14 06:52:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 06:49:16 2019
Response via : Initial Calibration

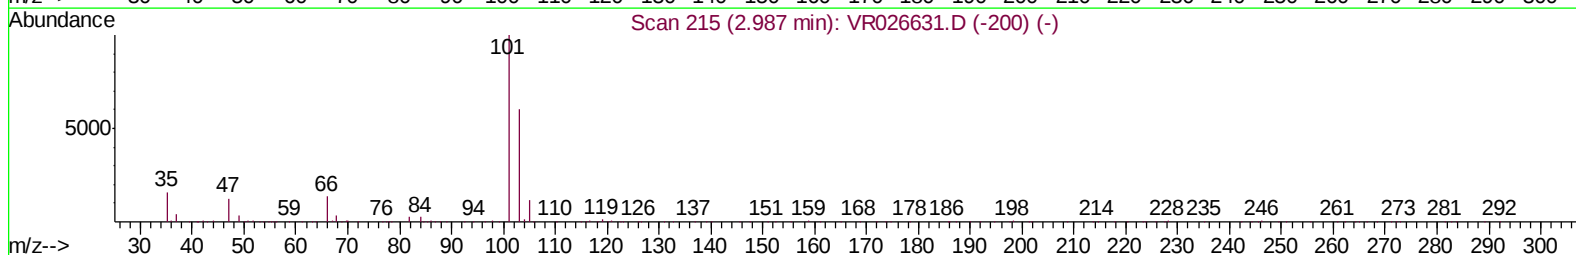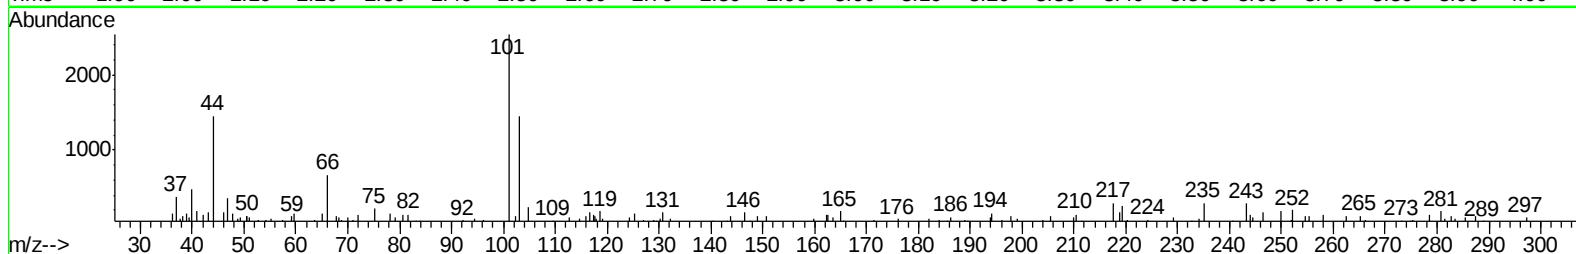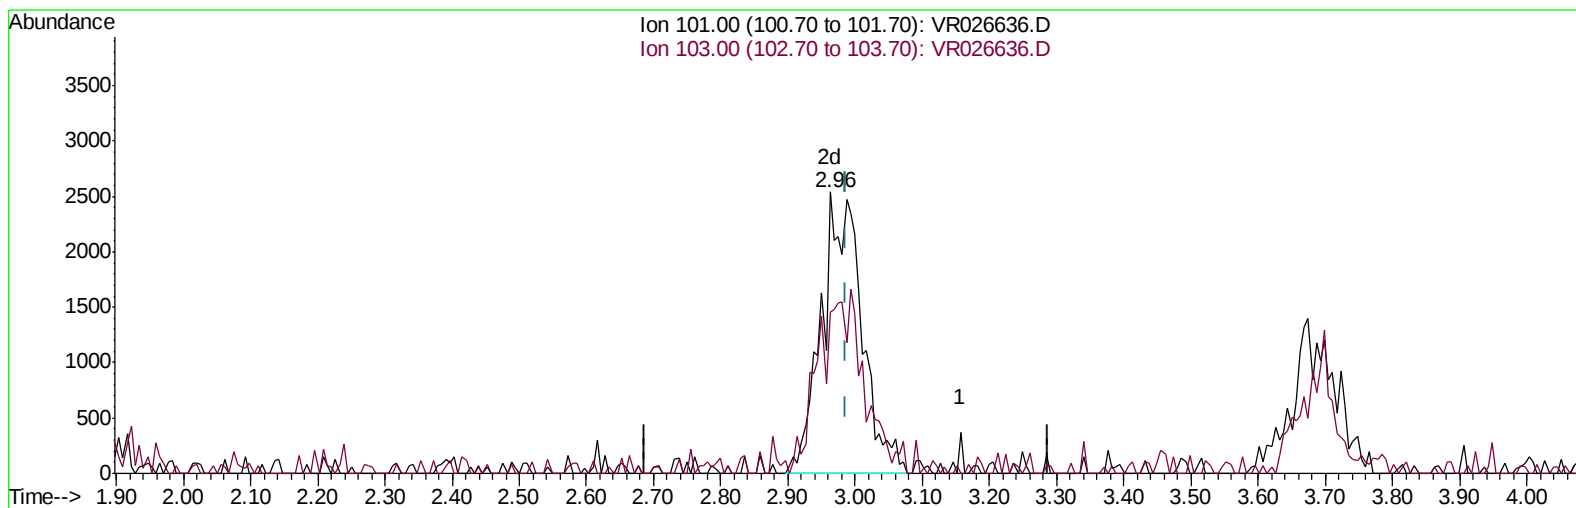

TIC: VR026636.D

(9) Trichlorofluoromethane (T)

2.963min (-0.024) 0.32ug/L m

response 10583

Ion	Exp%	Act%
101.00	100	100
103.00	63.60	1.12#
0.00	0.00	0.00
0.00	0.00	0.00




Data File : VR026636.D
Acq On : 13 Sep 2019 17:20
Operator : SY/MD
Sample : MDL02
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL02

Manual Integrations
APPROVED

MMDadoda
9/16/2019 12:45:01 AM

Quant Time: Sep 14 06:52:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 06:49:16 2019
Response via : Initial Calibration

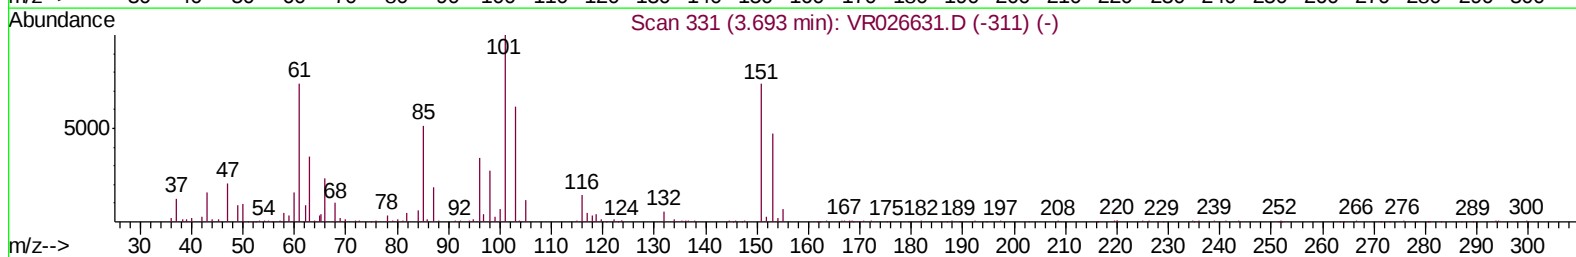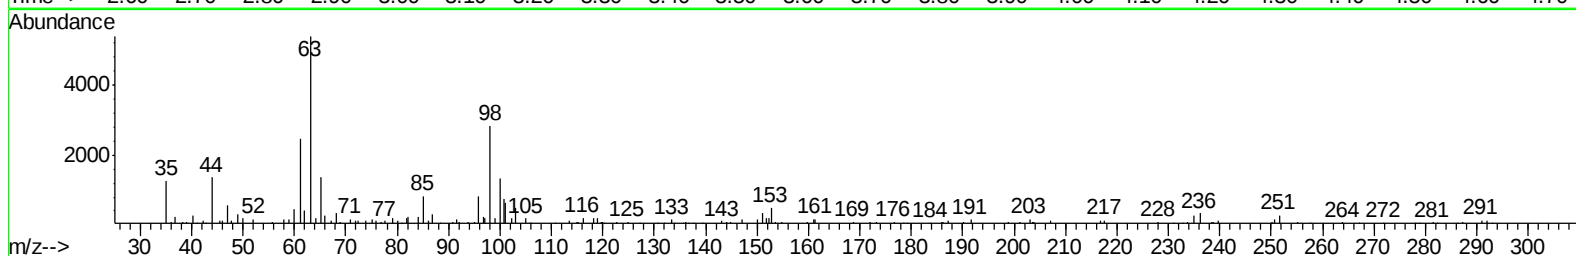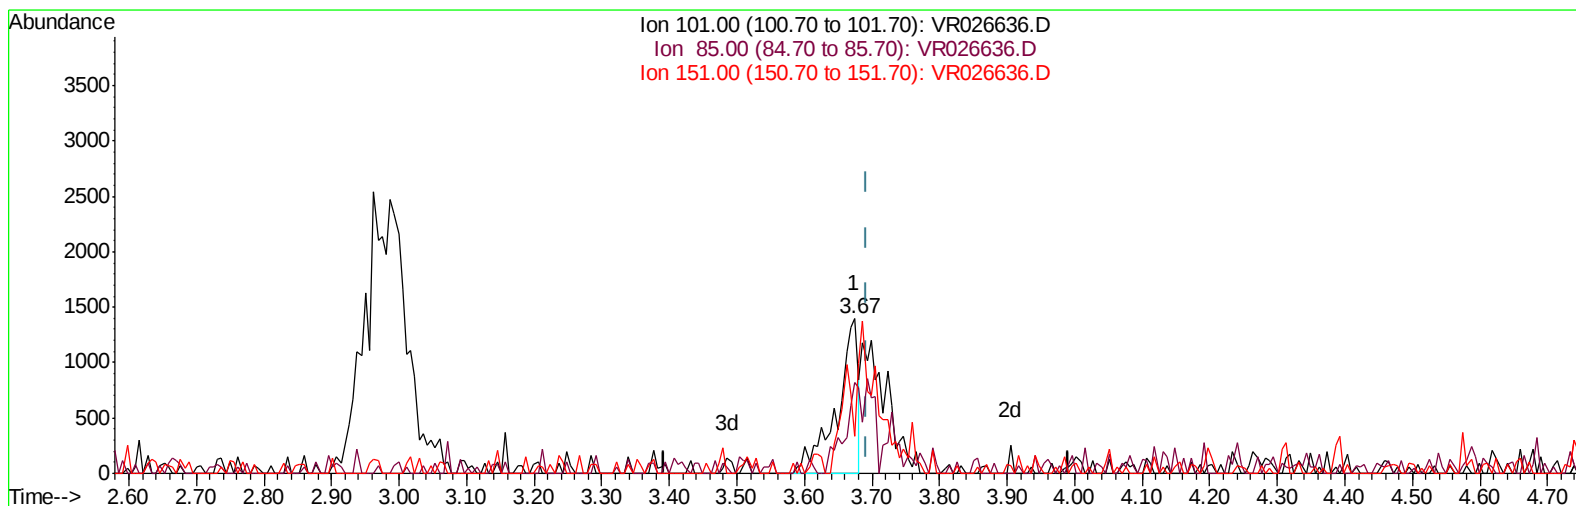

TIC: VR026636.D

(10) 1,1,2-Trichloro-1,2,2-trifluoroethane (T)

3.674min (-0.018) 0.21ug/L

response 3045

Ion	Exp%	Act%
101.00	100	100
85.00	49.60	48.21
151.00	73.00	39.38#
0.00	0.00	0.00




Data File : VR026636.D
Acq On : 13 Sep 2019 17:20
Operator : SY/MD
Sample : MDL02
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL02

Manual Integrations
APPROVED

MMDadoda
9/16/2019 12:45:01 AM

Quant Time: Sep 14 06:52:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 06:49:16 2019
Response via : Initial Calibration

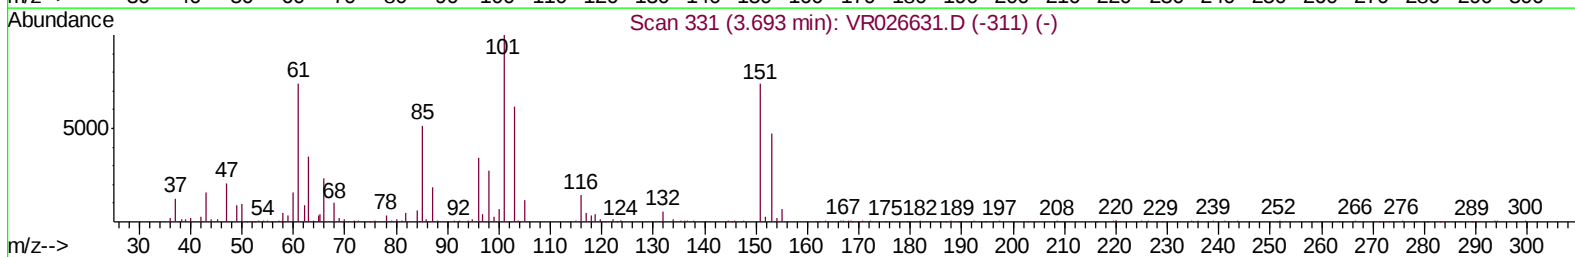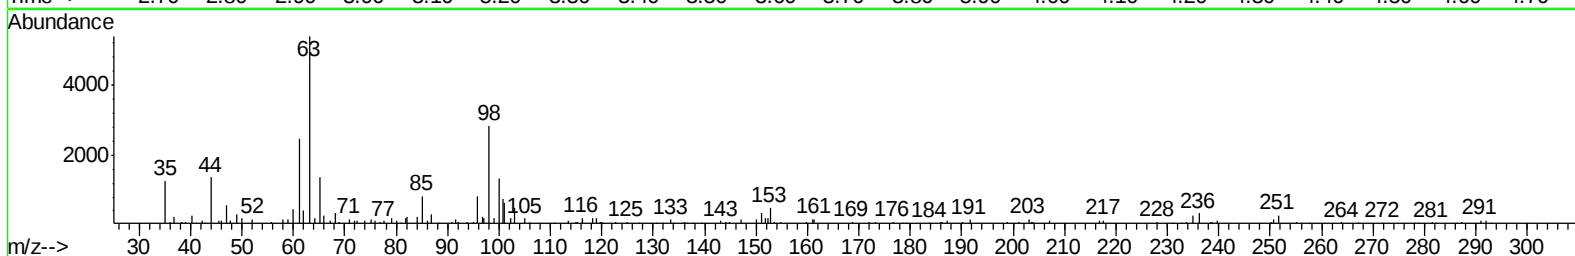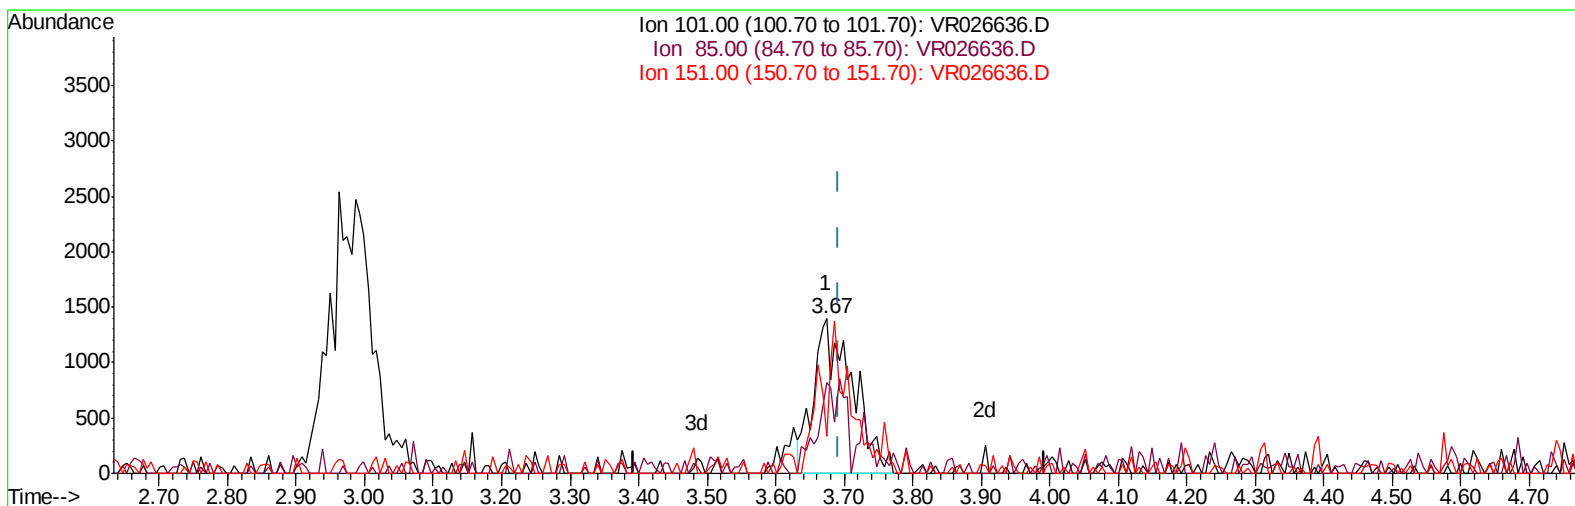

TIC: VR026636.D

(10) 1,1,2-Trichloro-1,2,2-trifluoroethane (T)

3.674min (-0.018) 0.39ug/L m

response 5529

Ion	Exp%	Act%
101.00	100	100
85.00	49.60	26.55#
151.00	73.00	21.69#
0.00	0.00	0.00




Data File : VR026636.D
Acq On : 13 Sep 2019 17:20
Operator : SY/MD
Sample : MDL02
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL02

Manual Integrations
APPROVED

MMDadoda
9/16/2019 12:45:01 AM

Quant Time: Sep 14 06:52:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 06:49:16 2019
Response via : Initial Calibration

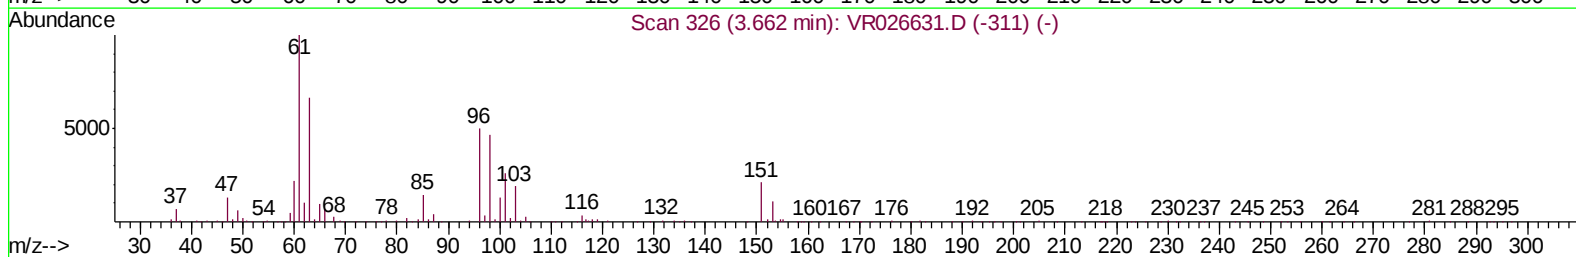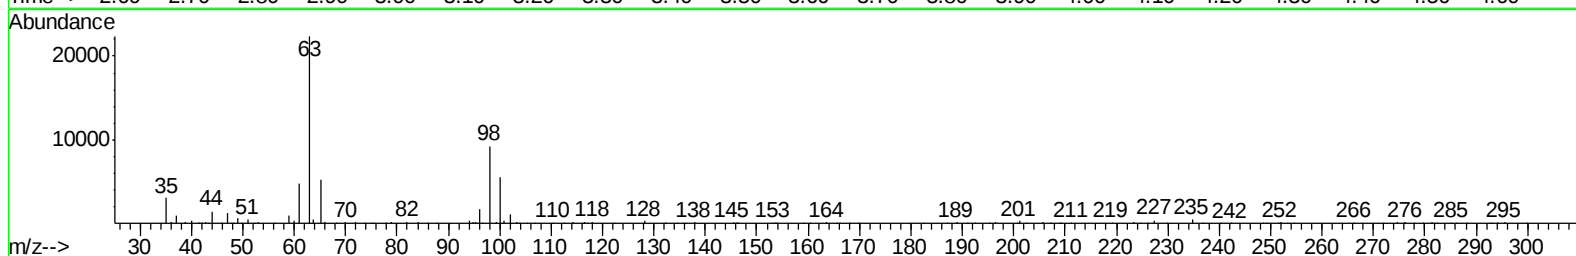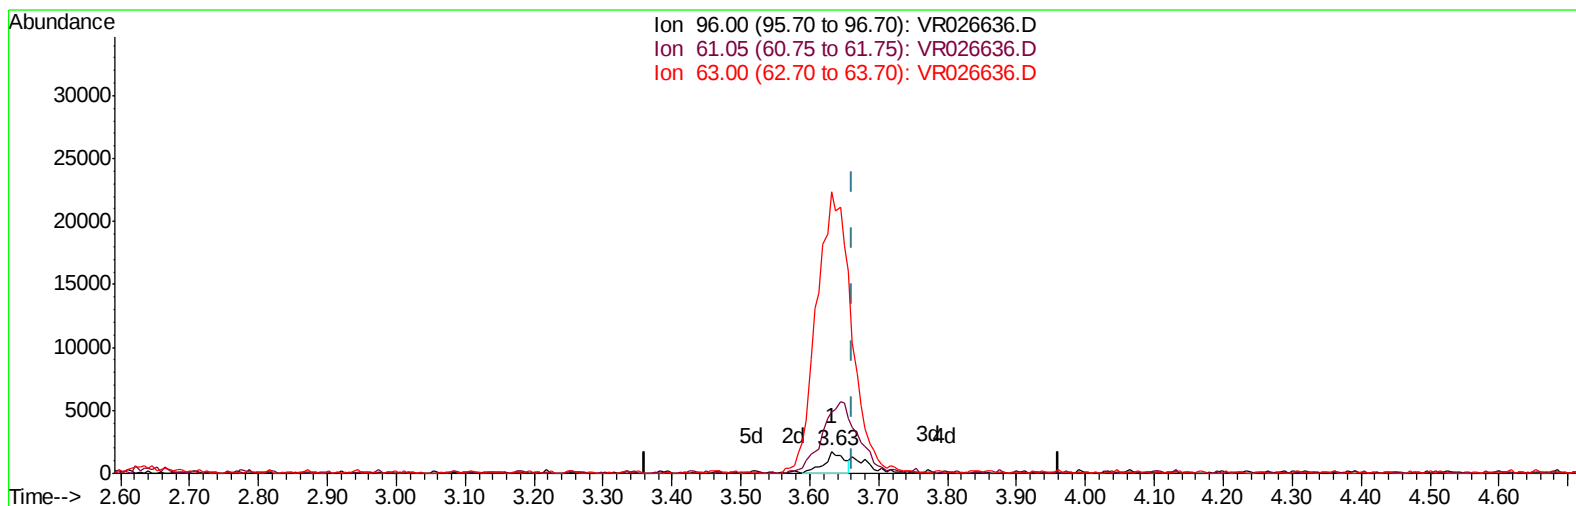

TIC: VR026636.D

(12) 1,1-Dichloroethene (T)

3.632min (-0.031) 0.25ug/L

response 3515

Ion	Exp%	Act%
96.00	100	100
61.05	204.70	260.33
63.00	160.80	1203.44#
0.00	0.00	0.00




Data File : VR026636.D
Acq On : 13 Sep 2019 17:20
Operator : SY/MD
Sample : MDL02
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL02

Manual Integrations
APPROVED

MMDadoda
9/16/2019 12:45:01 AM

Quant Time: Sep 14 06:52:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 06:49:16 2019
Response via : Initial Calibration

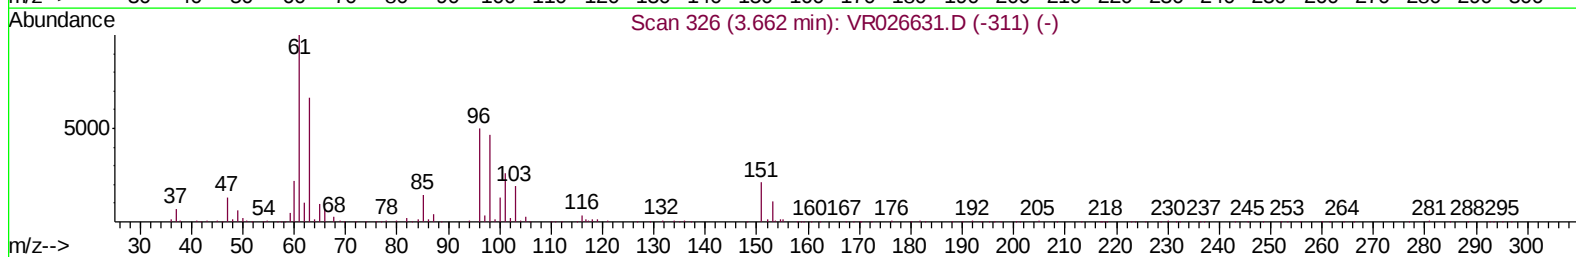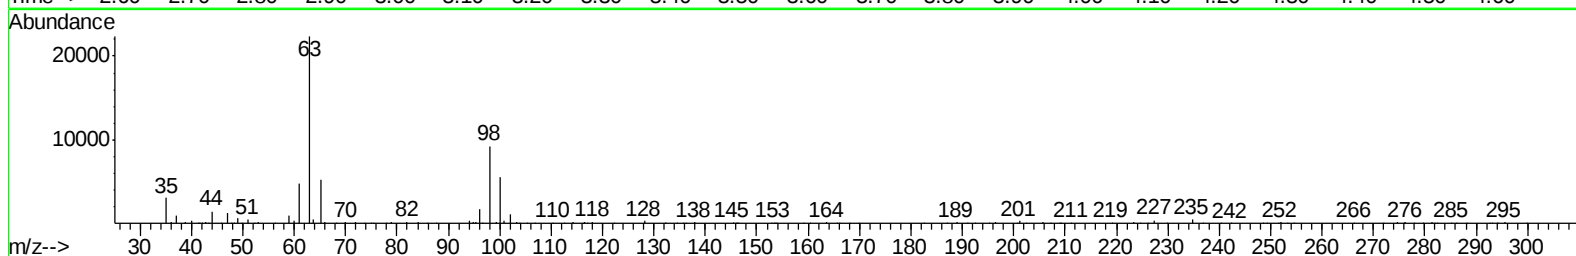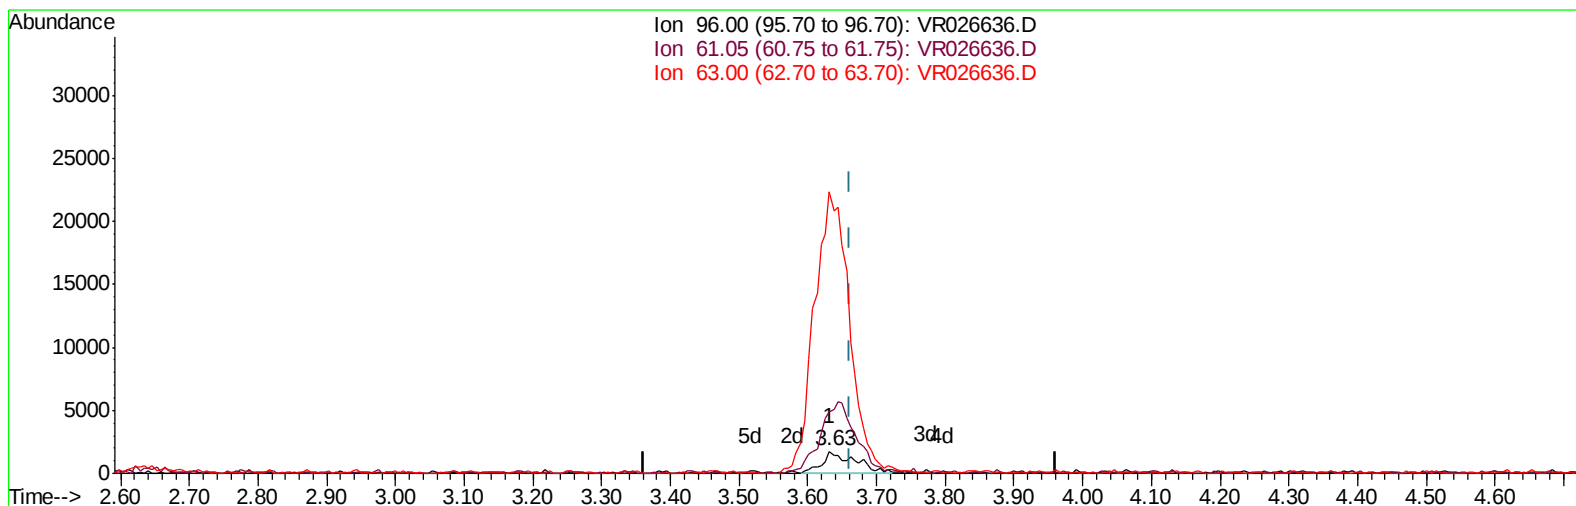

TIC: VR026636.D

(12) 1,1-Dichloroethene (T)
3.632min (-0.031) 0.42ug/L m
response 5883

Ion	Exp%	Act%
96.00	100	100
61.05	204.70	276.87#
63.00	160.80	1279.91#
0.00	0.00	0.00




Data File : VR026636.D
Acq On : 13 Sep 2019 17:20
Operator : SY/MD
Sample : MDL02
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL02

Manual Integrations
APPROVED

MMDadoda
9/16/2019 12:45:01 AM

Quant Time: Sep 14 06:52:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 06:49:16 2019
Response via : Initial Calibration

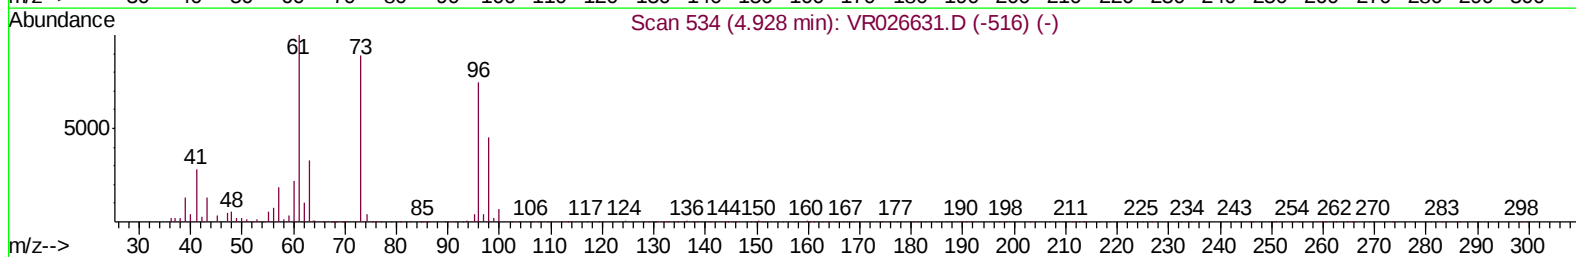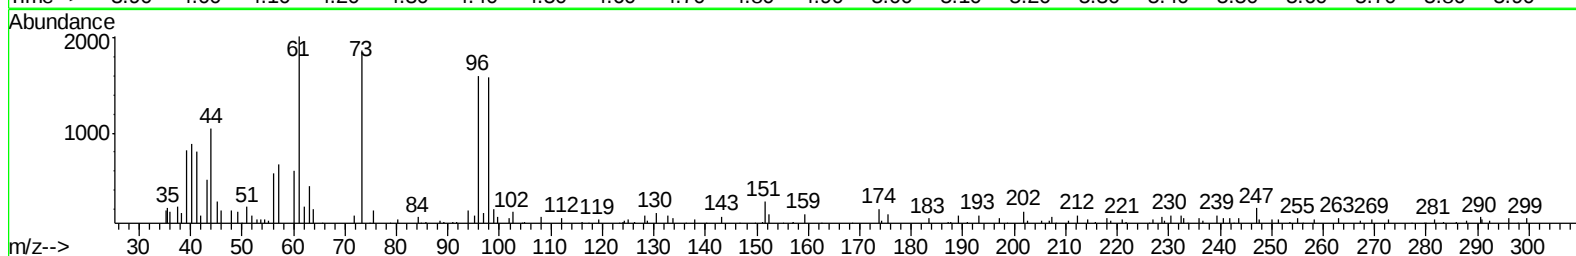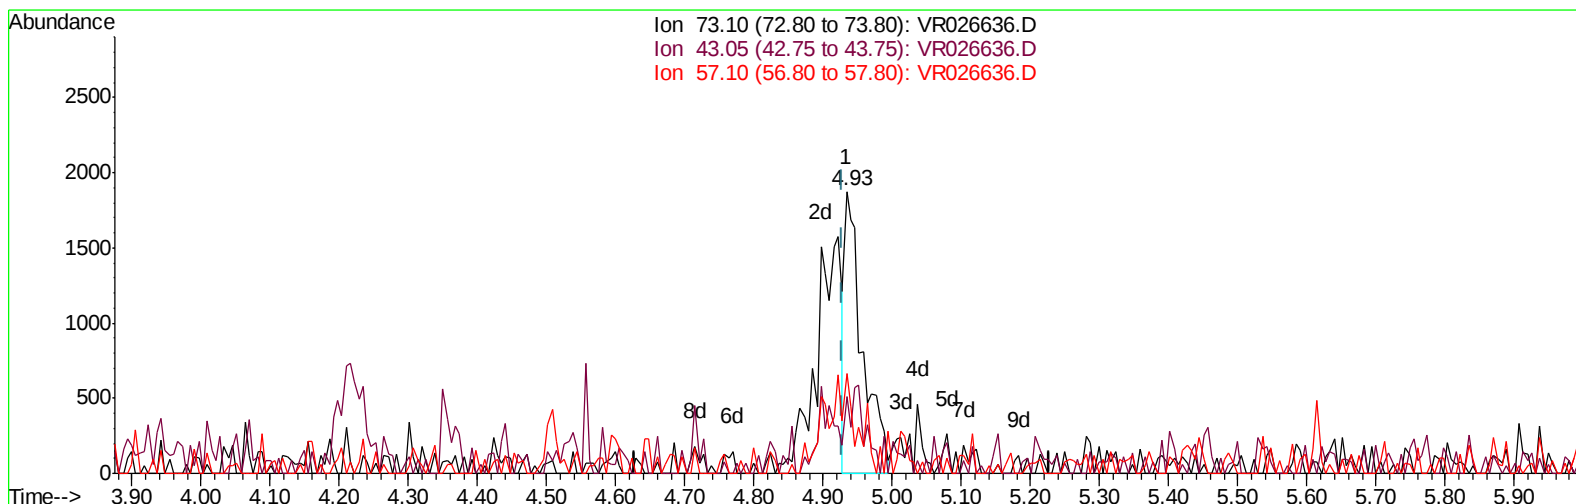

TIC: VR026636.D

(17) Methyl tert-butyl Ether (T)

4.934min (+0.006) 0.11ug/L

response 3305

Ion	Exp%	Act%
73.10	100	100
43.05	18.40	30.95#
57.10	23.60	18.58#
0.00	0.00	0.00




Data File : VR026636.D
Acq On : 13 Sep 2019 17:20
Operator : SY/MD
Sample : MDL02
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL02

Manual Integrations
APPROVED

MMDadoda
9/16/2019 12:45:01 AM

Quant Time: Sep 14 06:52:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 06:49:16 2019
Response via : Initial Calibration

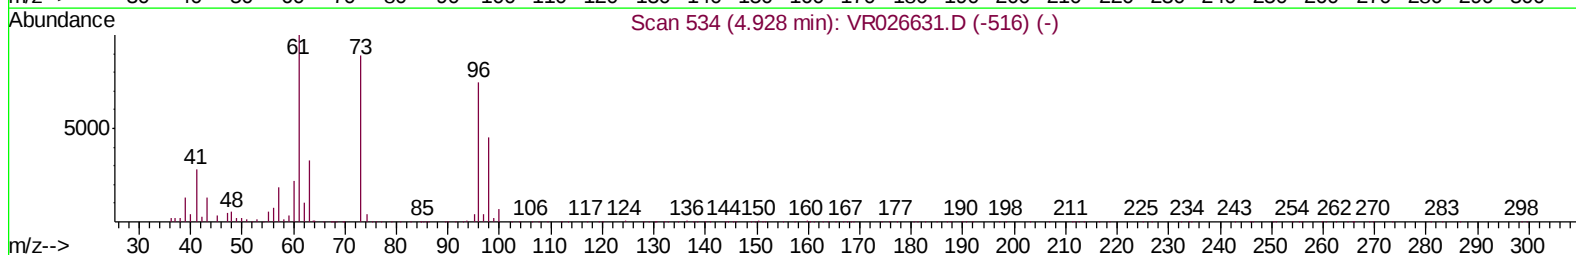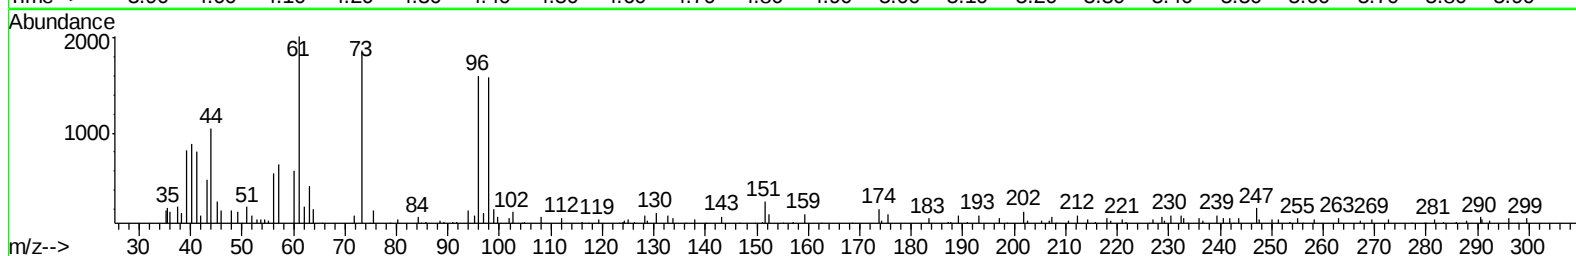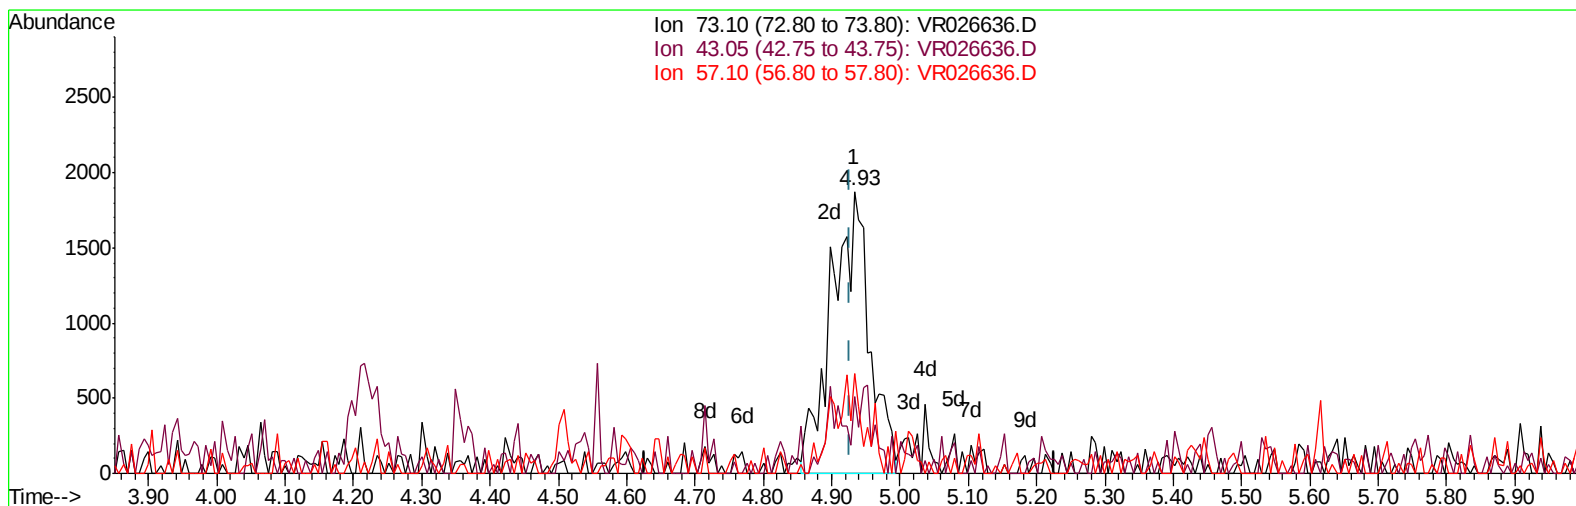

TIC: VR026636.D

(17) Methyl tert-butyl Ether (T)

4.934min (+0.006) 0.24ug/L m

response 7239

Ion	Exp%	Act%
73.10	100	100
43.05	18.40	14.13#
57.10	23.60	8.48#
0.00	0.00	0.00

Data File : VR026636.D

Acq On : 13 Sep 2019 17:20

Operator : SY/MD

Sample : MDL02

Misc : 25mL/MSVOA_R/WATER

ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL02

Manual Integrations
APPROVED

MMDadoda
9/16/2019 12:45:01 AM




Quant Time: Sep 14 06:52:53 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091219WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Sat Sep 14 06:49:16 2019

Response via : Initial Calibration

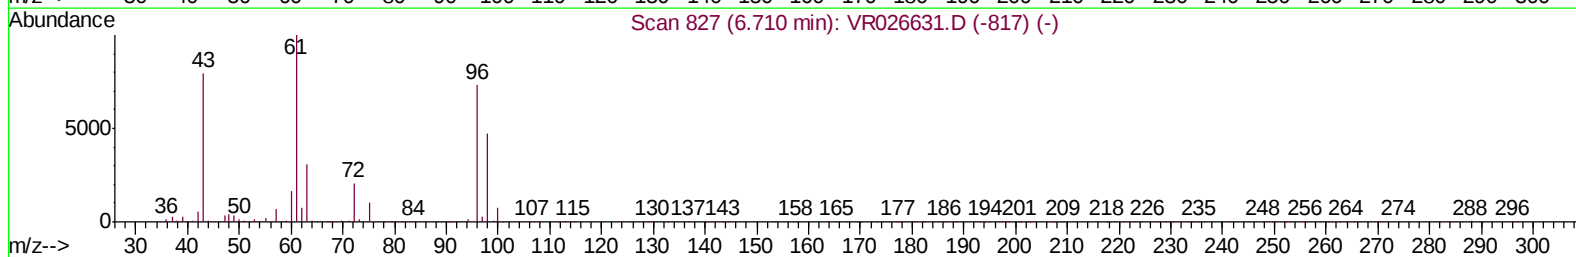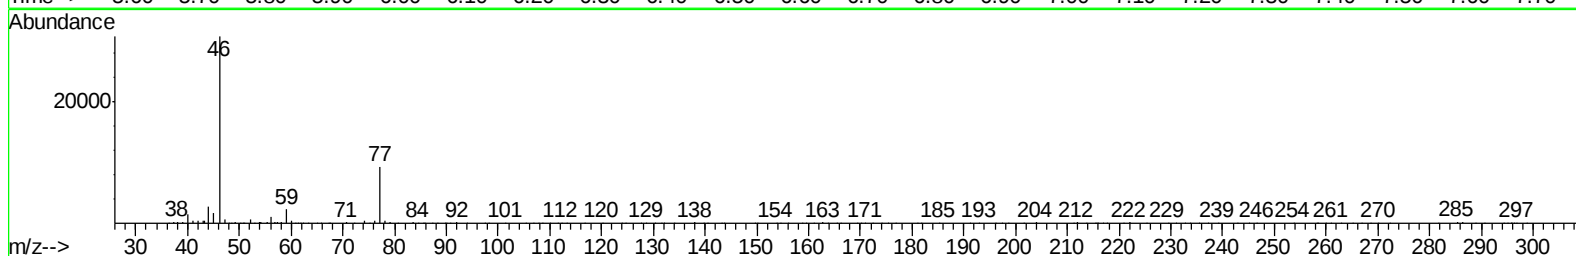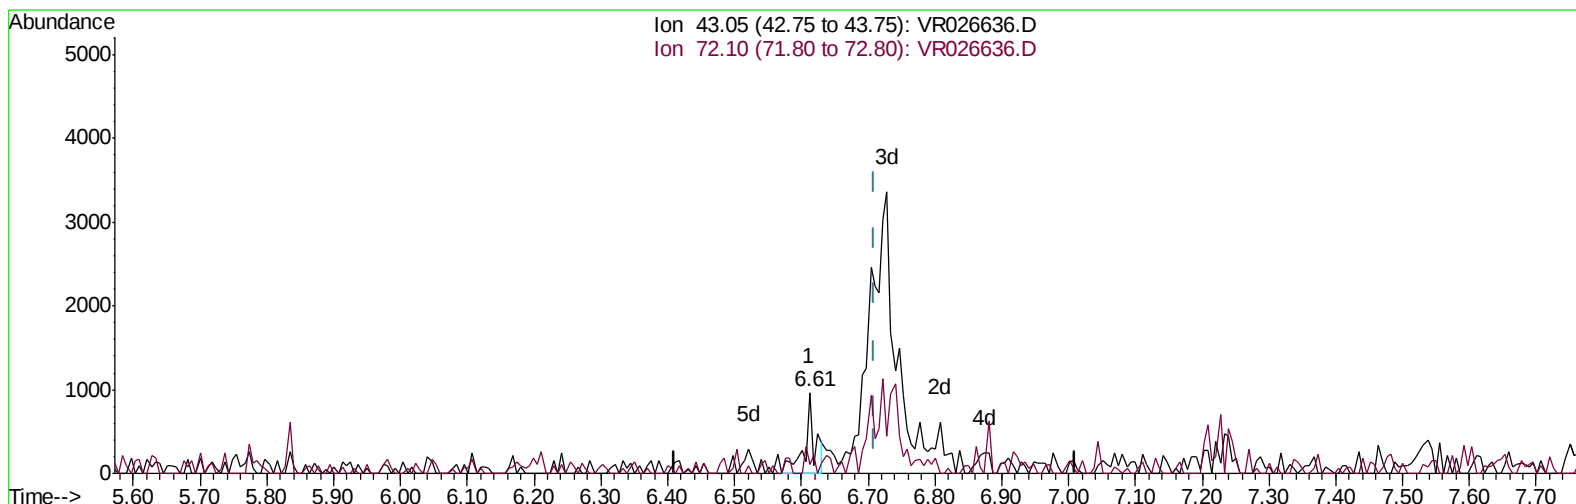

TIC: VR026636.D

(21) 2-Butanone (T)

6.613min (-0.097) 0.40ug/L

response 1057

Ion	Exp%	Act%
43.05	100	100
72.10	30.10	21.76
0.00	0.00	0.00
0.00	0.00	0.00




Data File : VR026636.D
Acq On : 13 Sep 2019 17:20
Operator : SY/MD
Sample : MDL02
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL02

Manual Integrations
APPROVED

MMDadoda
9/16/2019 12:45:01 AM

Quant Time: Sep 14 06:52:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 06:49:16 2019
Response via : Initial Calibration

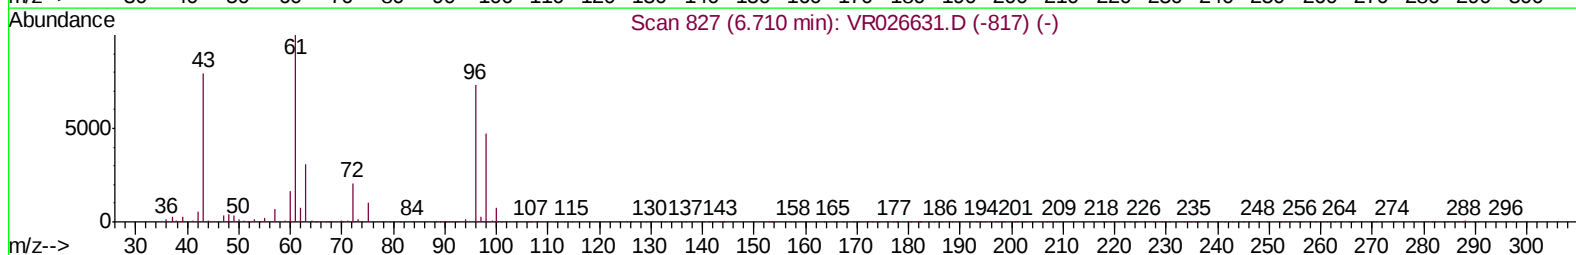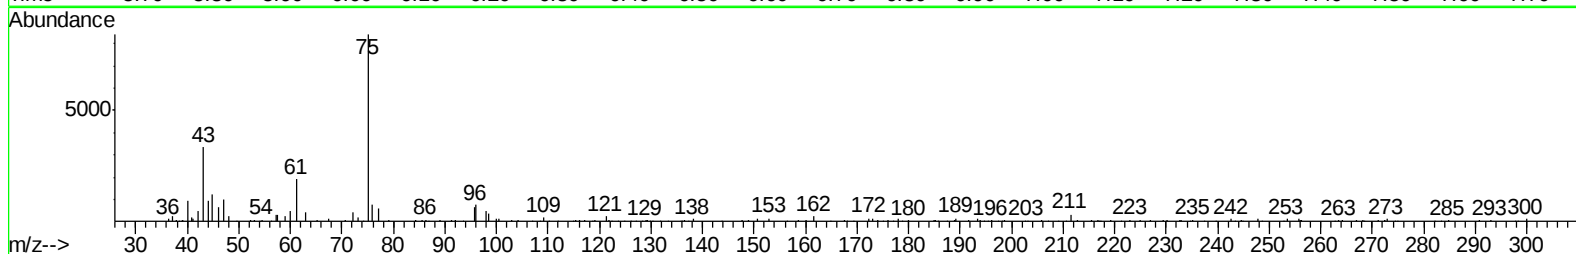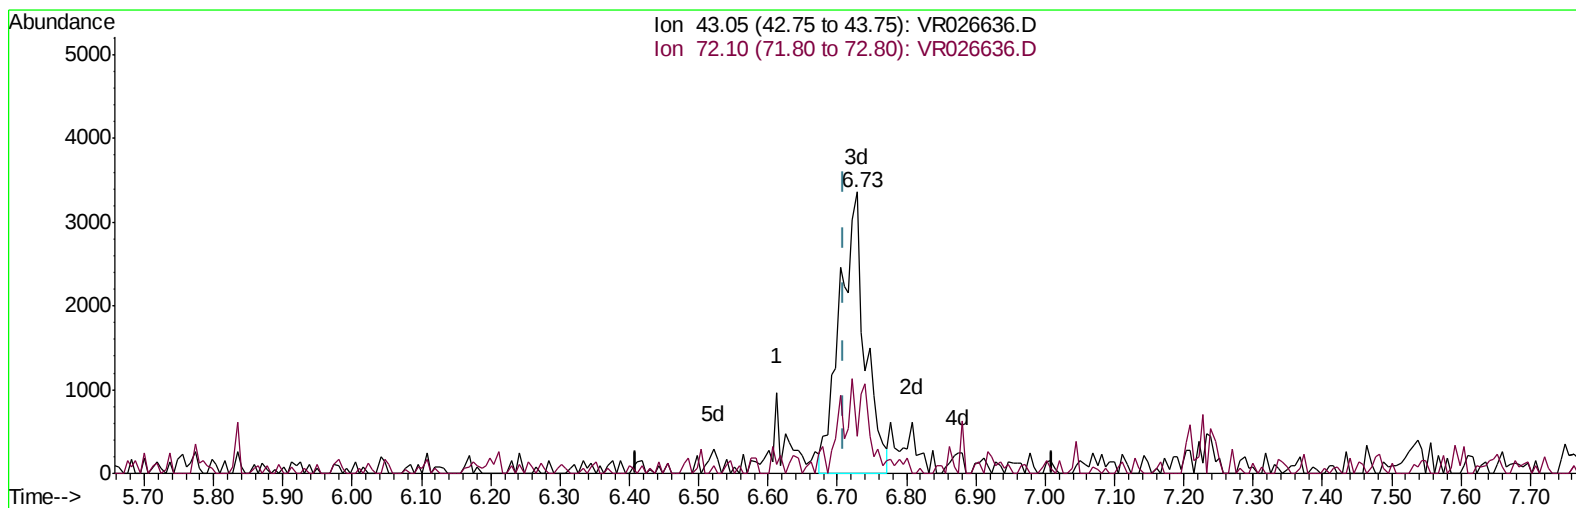

TIC: VR026636.D

(21) 2-Butanone (T)
6.728min (+0.018) 3.23ug/L m
response 8421

Ion	Exp%	Act%
43.05	100	100
72.10	30.10	2.73#
0.00	0.00	0.00
0.00	0.00	0.00




Data File : VR026636.D
Acq On : 13 Sep 2019 17:20
Operator : SY/MD
Sample : MDL02
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL02

Manual Integrations
APPROVED

MMDadoda
9/16/2019 12:45:01 AM

Quant Time: Sep 14 06:52:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 06:49:16 2019
Response via : Initial Calibration

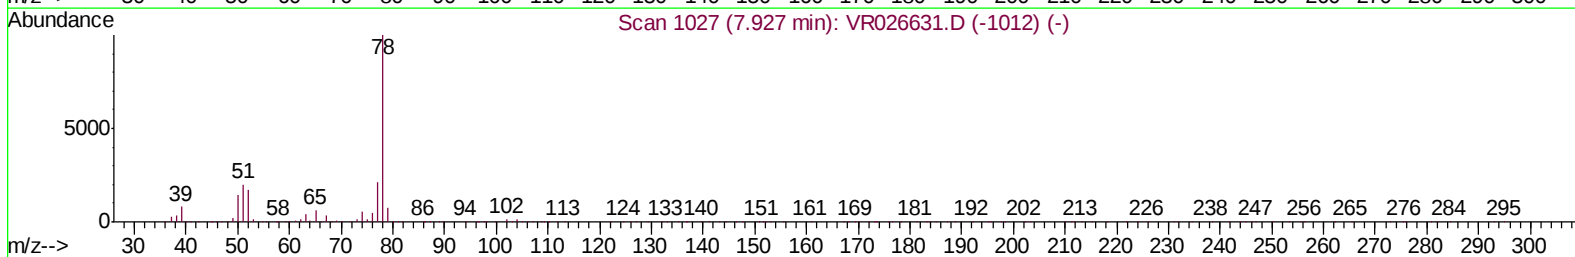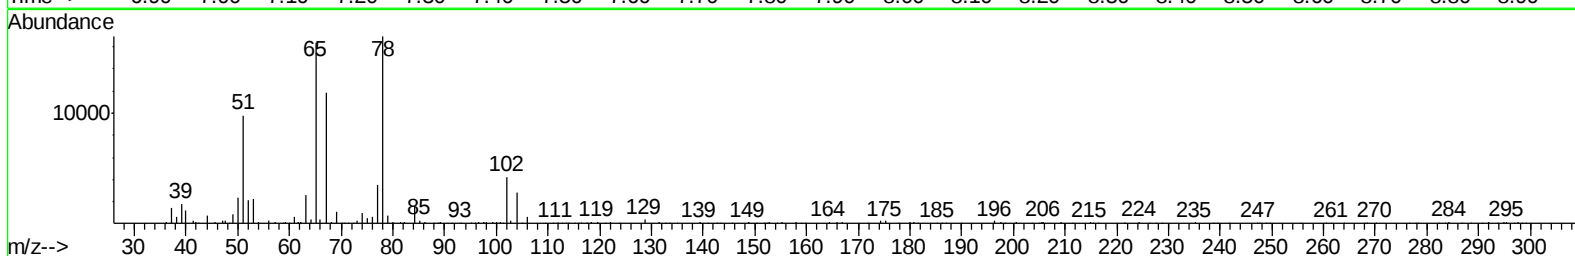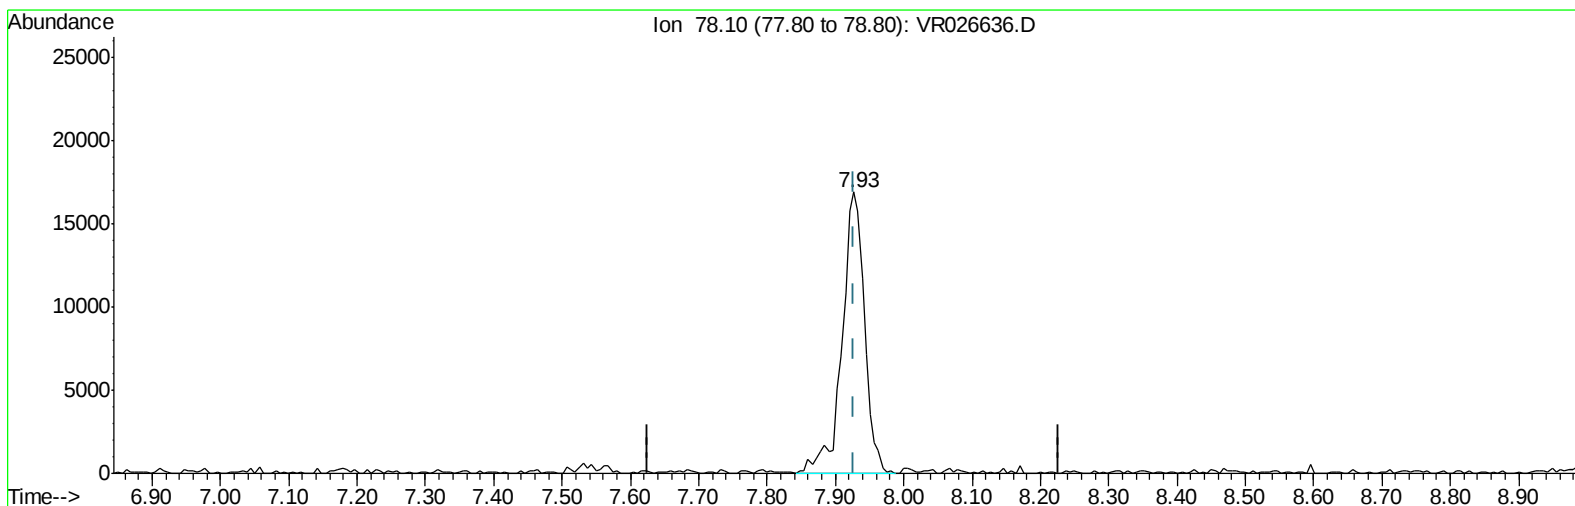

TIC: VR026636.D

(33) Benzene (T)

7.927min (-0.000) 0.34ug/L

response 38598

Ion	Exp%	Act%
78.10	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data File : VR026636.D
Acq On : 13 Sep 2019 17:20
Operator : SY/MD
Sample : MDL02
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL02

Manual Integrations
APPROVED

MMDadoda
9/16/2019 12:45:01 AM

Quant Time: Sep 14 06:52:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 06:49:16 2019
Response via : Initial Calibration

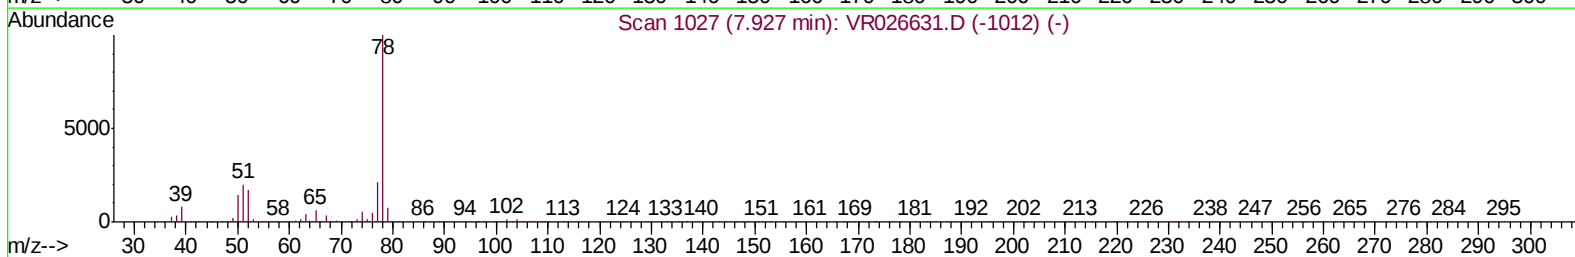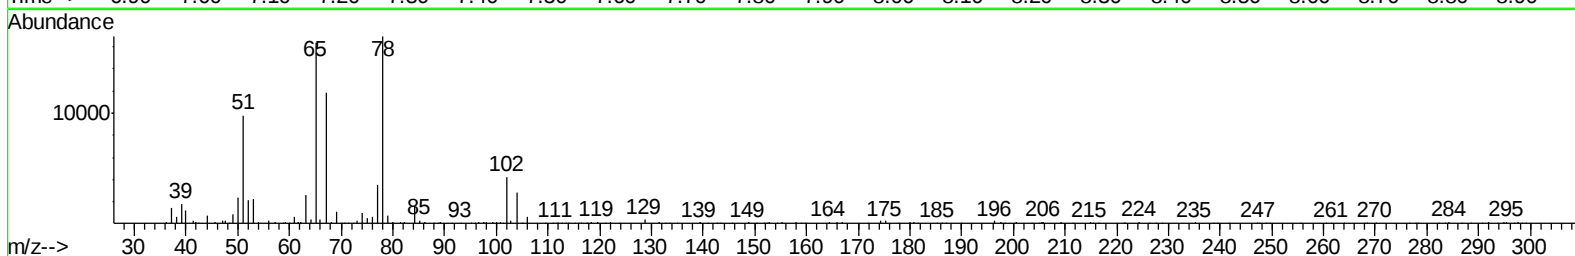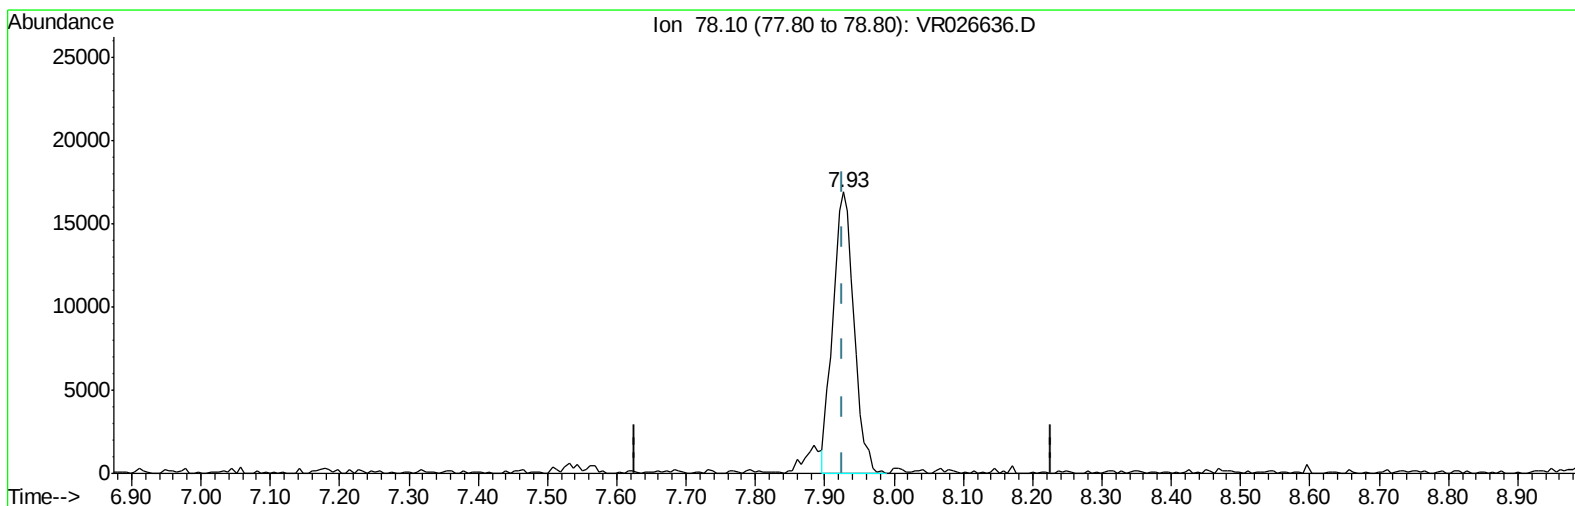

TIC: VR026636.D

(33) Benzene (T)

7.927min (-0.000) 0.31ug/L m

response 35566

Ion	Exp%	Act%
78.10	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data File : VR026636.D
Acq On : 13 Sep 2019 17:20
Operator : SY/MD
Sample : MDL02
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL02

Manual Integrations
APPROVED

MMDadoda
9/16/2019 12:45:01 AM

Quant Time: Sep 14 06:52:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 06:49:16 2019
Response via : Initial Calibration

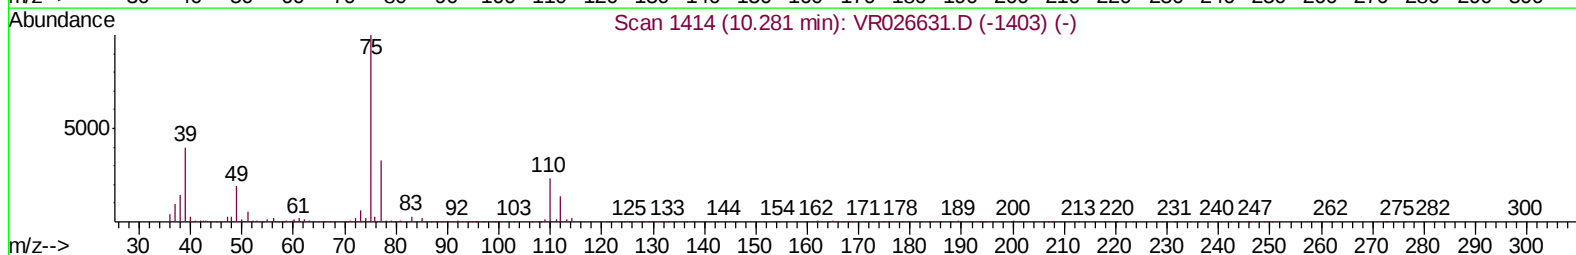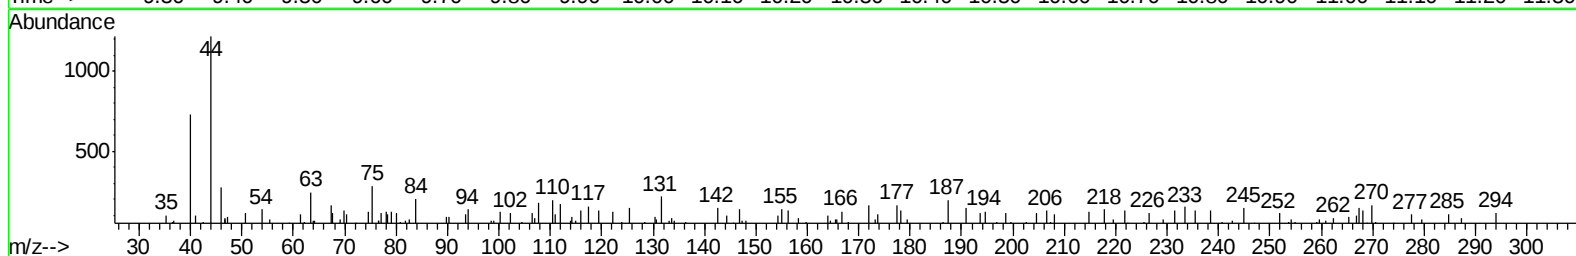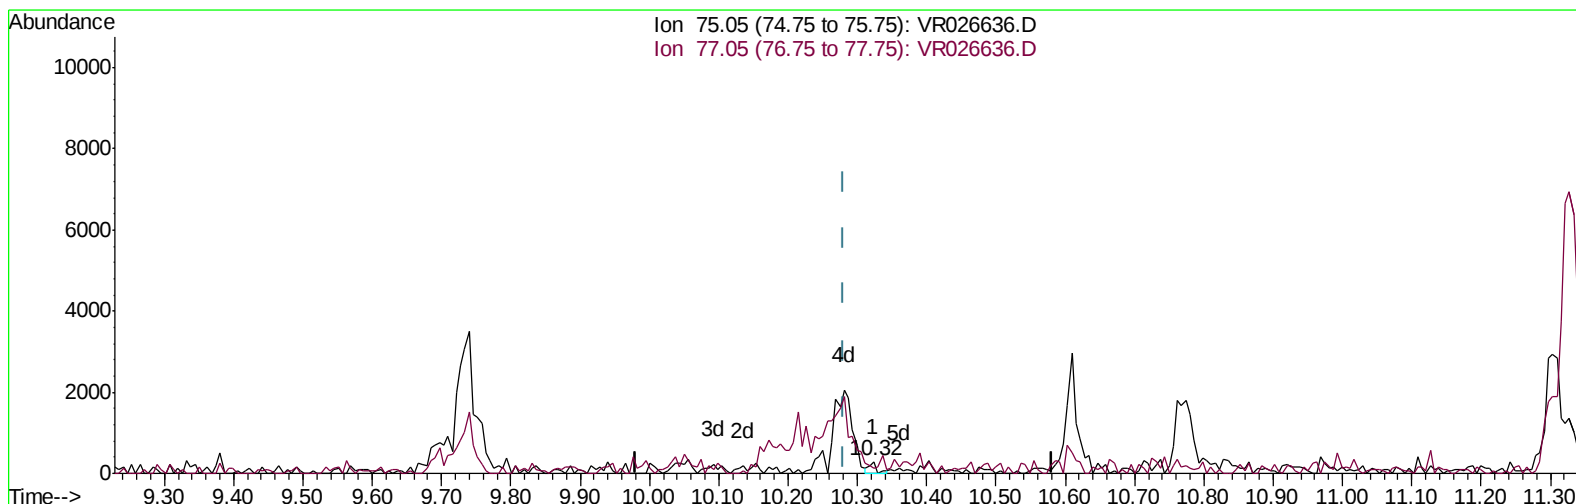

TIC: VR026636.D

(44) trans-1,3-Dichloropropene (T)

10.324min (+0.042) 0.01ug/L

response 219

Ion	Exp%	Act%
75.05	100	100
77.05	33.00	39.44
0.00	0.00	0.00
0.00	0.00	0.00




Data File : VR026636.D
Acq On : 13 Sep 2019 17:20
Operator : SY/MD
Sample : MDL02
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL02

Manual Integrations
APPROVED

MMDadoda
9/16/2019 12:45:01 AM

Quant Time: Sep 14 06:52:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 06:49:16 2019
Response via : Initial Calibration

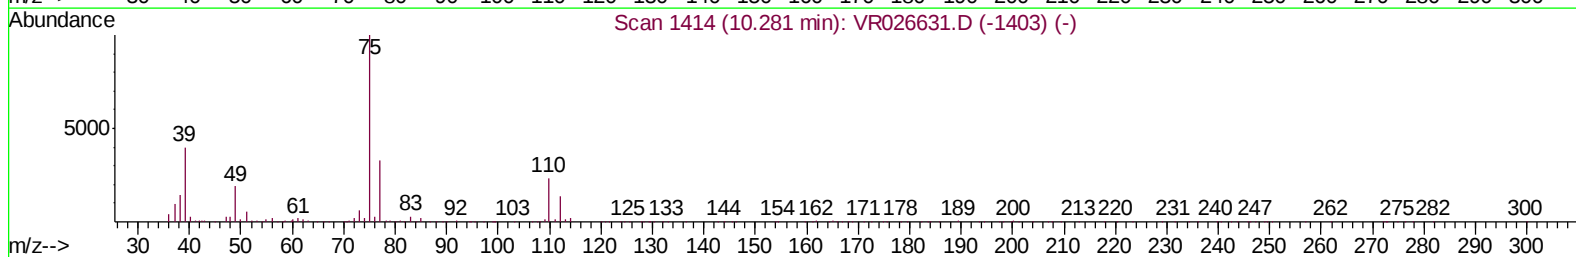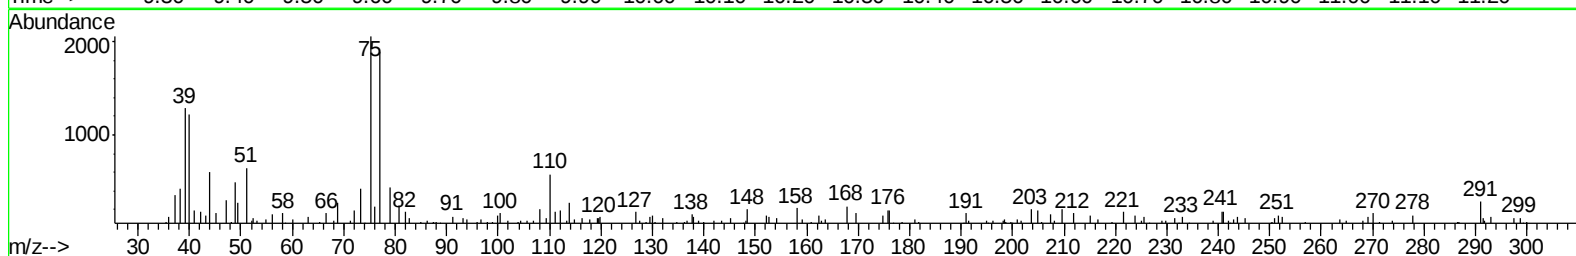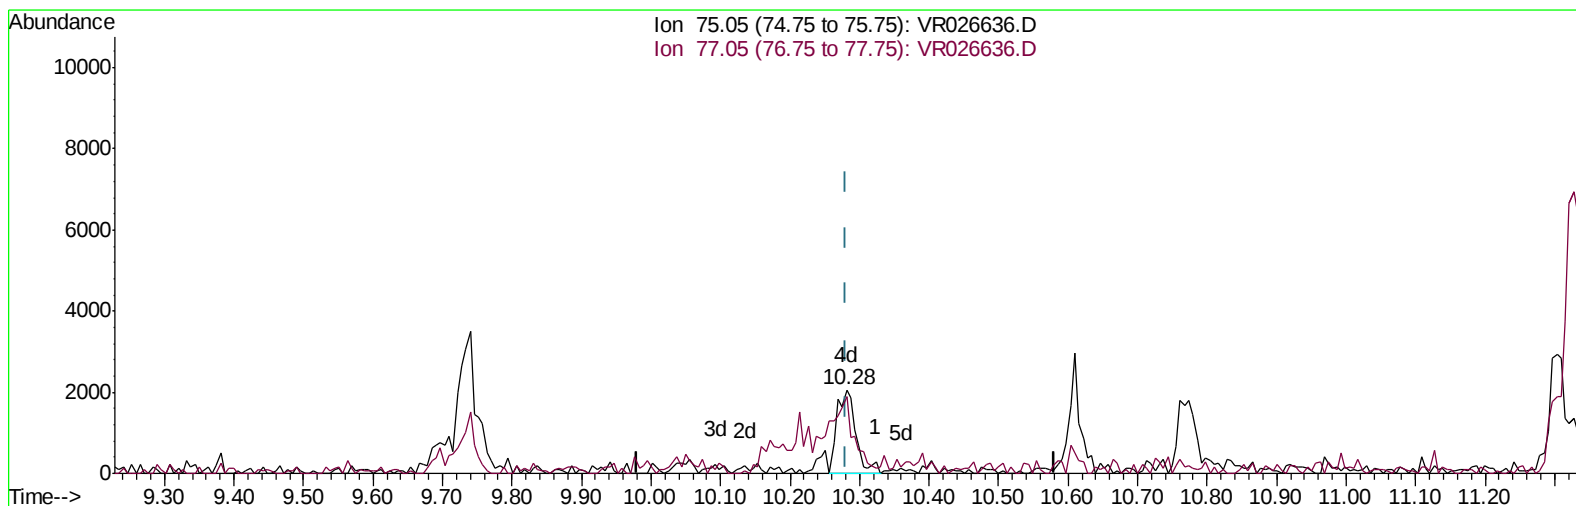

TIC: VR026636.D

(44) trans-1,3-Dichloropropene (T)

10.281min (-0.000) 0.25ug/L m

response 3904

Ion	Exp%	Act%
75.05	100	100
77.05	33.00	91.69#
0.00	0.00	0.00
0.00	0.00	0.00

Data File : VR026636.D

Acq On : 13 Sep 2019 17:20

Operator : SY/MD

Sample : MDL02

Misc : 25mL/MSVOA_R/WATER

ALS Vial : 8 Sample Multiplier: 1

Instrument :

MSVOA_R

ClientSampleId :

MDL02

Manual Integrations
APPROVED

MMDadoda
9/16/2019 12:45:01 AM




Quant Time: Sep 14 06:52:53 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091219WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Sat Sep 14 06:49:16 2019

Response via : Initial Calibration

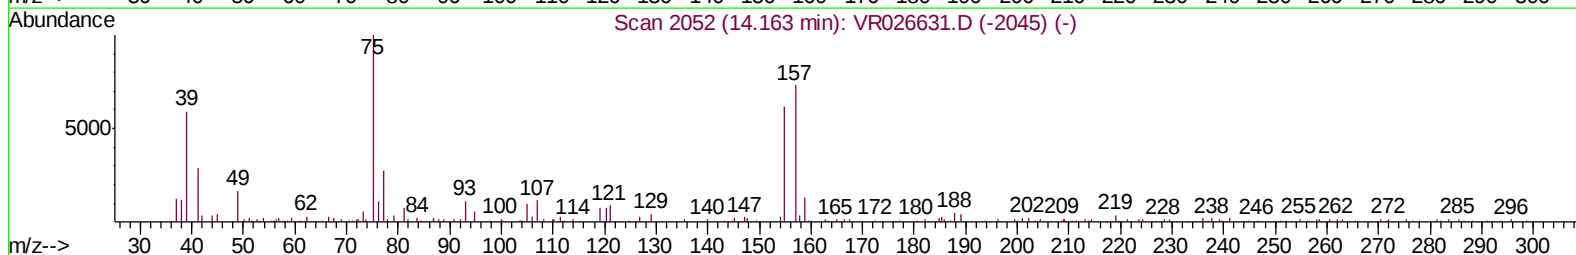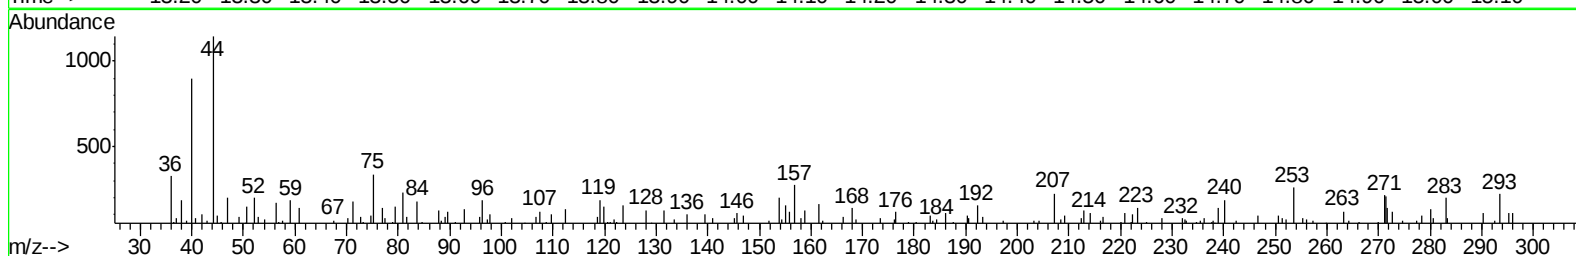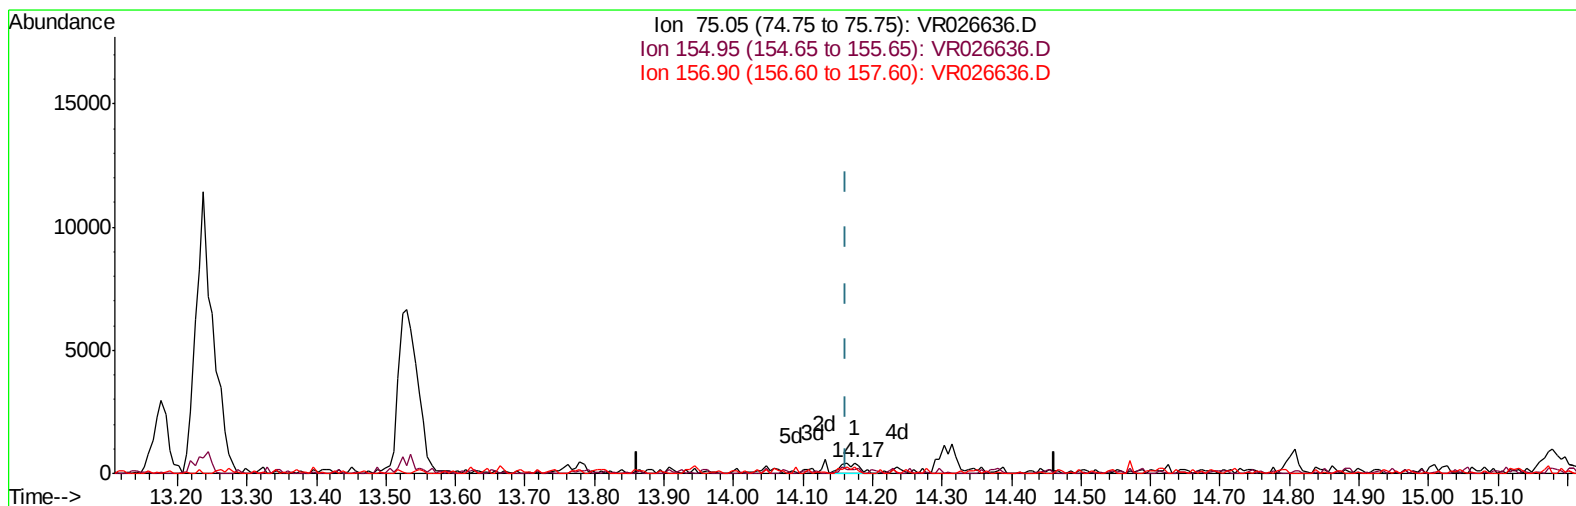

TIC: VR026636.D

(66) 1,2-Dibromo-3-chloropropane (T)

14.175min (+0.012) 0.43ug/L

response 752

Ion	Exp%	Act%
75.05	100	100
154.95	61.80	35.50#
156.90	81.50	63.11#
0.00	0.00	0.00

Data File : VR026636.D

Acq On : 13 Sep 2019 17:20

Operator : SY/MD

Sample : MDL02

Misc : 25mL/MSVOA_R/WATER

ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL02

Manual Integrations
APPROVED

MMDadoda
9/16/2019 12:45:01 AM




Quant Time: Sep 14 06:52:53 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091219WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Sat Sep 14 06:49:16 2019

Response via : Initial Calibration

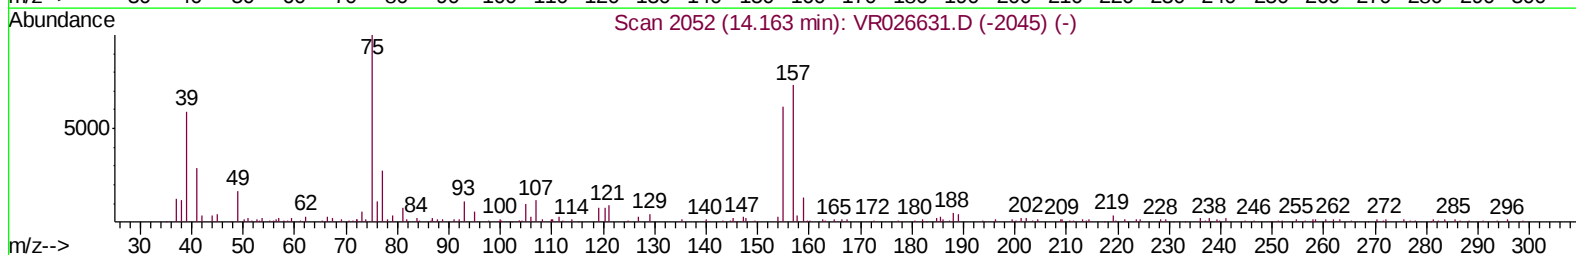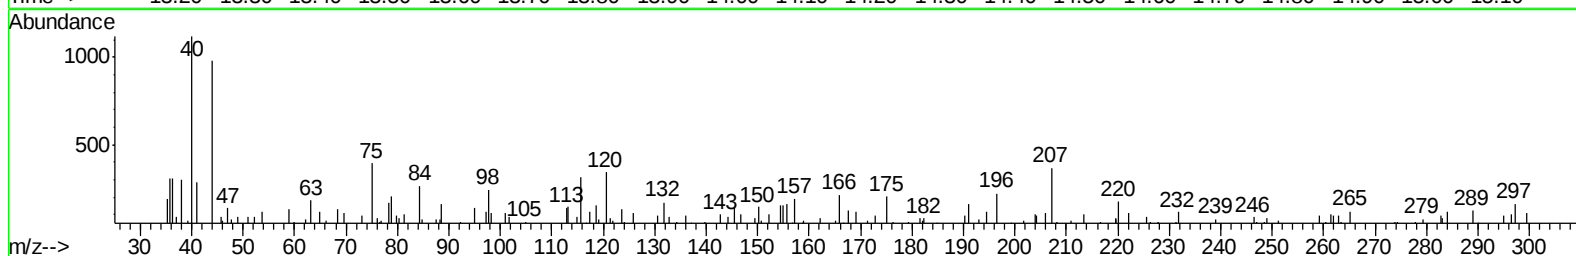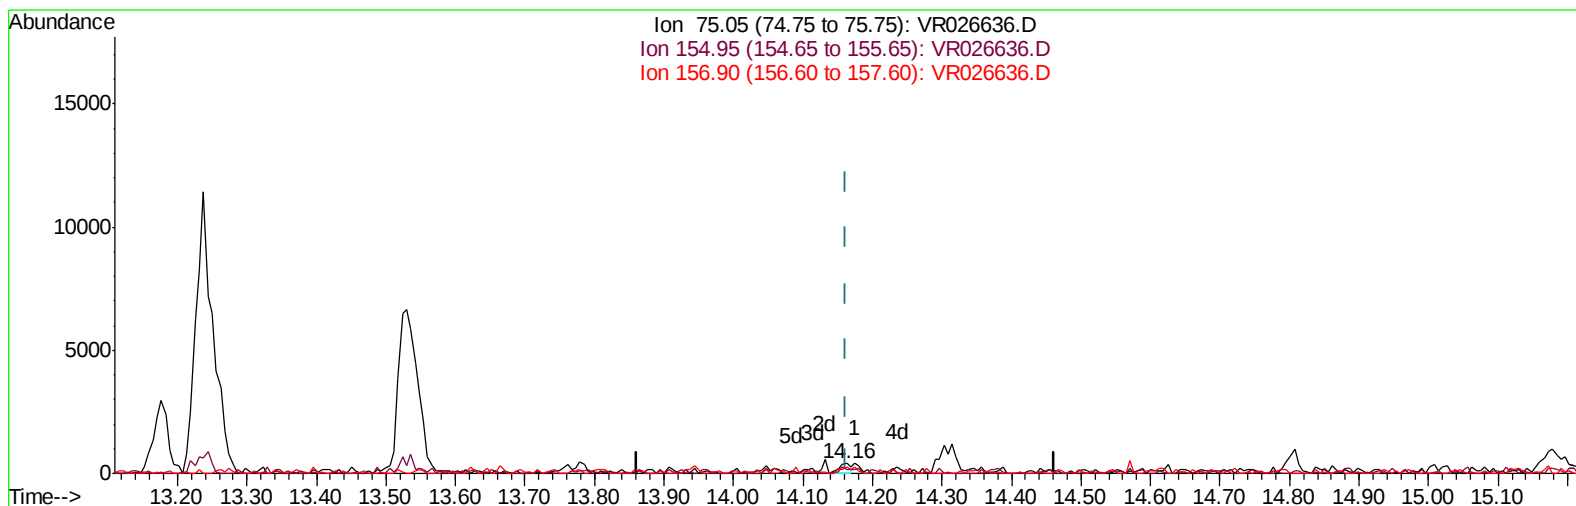

TIC: VR026636.D

(66) 1,2-Dibromo-3-chloropropane (T)

14.162min (-0.000) 0.26ug/L m

response 448

Ion	Exp%	Act%
75.05	100	100
154.95	61.80	38.23#
156.90	81.50	49.11#
0.00	0.00	0.00

Data File : VR026636.D
Acq On : 13 Sep 2019 17:20
Operator : SY/MD
Sample : MDL02
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL02

Manual Integrations
APPROVED

MMDadoda
9/16/2019 12:45:01 AM

Quant Time: Sep 14 07:08:51 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 06:49:16 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.48	114	318944	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.30	117	258208	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.24	152	115587	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.19	65	38458	4.39	ug/L	0.01
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.80%
7) Chloroethane-d5	2.63	69	37409	4.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.60%
11) 1,1-Dichloroethene-d2	3.63	63	79503	3.28	ug/L	-0.02
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.60%
20) 2-Butanone-d5	6.62	46	91507	48.14	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.28%
24) Chloroform-d	7.22	84	171699	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
26) 1,2-Dichloroethane-d4	7.91	65	57241	5.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.60%
32) Benzene-d6	7.87	84	301965	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.80%
36) 1,2-Dichloropropane-d6	8.92	67	83341	4.89	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.80%
41) Toluene-d8	9.99	98	224469	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.00%
43) trans-1,3-Dichloropropene-	10.25	79	16329	4.20	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.00%
46) 2-Hexanone-d5	10.61	63	57513	49.15	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.30%
57) 1,1,2,2-Tetrachloroethane-	12.37	84	45205	4.99	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.80%
64) 1,2-Dichlorobenzene-d4	13.53	152	76698	5.23	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.60%

Target Compounds

					Qvalue
2) Dichlorodifluoromethane	1.85	85	11445	0.317 ug/L	99
3) Chloromethane	2.06	50	6566	0.349 ug/L #	81
5) Vinyl chloride	2.20	62	5353	0.284 ug/L #	64
6) Bromomethane	2.54	94	4552	0.384 ug/L #	61
8) Chloroethane	2.65	64	4327m	0.398 ug/L	
9) Trichlorofluoromethane	2.96	101	10583m	0.324 ug/L	
10) 1,1,2-Trichloro-1,2,2-trif	3.67	101	5529m	0.387 ug/L	
12) 1,1-Dichloroethene	3.63	96	5883m	0.418 ug/L	
13) Acetone	3.74	43	5677	3.972 ug/L	85
14) Carbon disulfide	3.98	76	15469	0.257 ug/L #	86
15) Methyl Acetate	4.22	43	1906	0.318 ug/L #	64
16) Methylene chloride	4.42	84	13694	0.468 ug/L	80
17) Methyl tert-butyl Ether	4.93	73	7239m	0.238 ug/L	
18) trans-1,2-Dichloroethene	4.92	96	9610	0.327 ug/L #	66
19) 1,1-Dichloroethane	5.72	63	17540	0.318 ug/L	98
21) 2-Butanone	6.73	43	8421m	3.225 ug/L	
22) cis-1,2-Dichloroethene	6.69	96	8313	0.295 ug/L	84

Data File : VR026636.D
Acq On : 13 Sep 2019 17:20
Operator : SY/MD
Sample : MDL02
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL02

Manual Integrations
APPROVED

MMDadoda
9/16/2019 12:45:01 AM

Quant Time: Sep 14 07:08:51 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 06:49:16 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)

23) Bromochloromethane	7.08	128	2595	0.331	ug/L #	61
25) Chloroform	7.25	83	22068	0.418	ug/L	86
27) 1,2-Dichloroethane	8.02	62	7466	0.402	ug/L #	91
29) 1,1,1-Trichloroethane	7.45	97	12100	0.291	ug/L	96
30) Cyclohexane	7.54	56	8316	0.188	ug/L #	84
31) Carbon tetrachloride	7.65	117	10736	0.305	ug/L	98
33) Benzene	7.93	78	35566m	0.311	ug/L	
34) Trichloroethene	8.73	95	8515	0.299	ug/L	88
35) Methylcyclohexane	8.98	83	10247	0.239	ug/L	93
37) 1,2-Dichloropropane	9.02	63	8396	0.363	ug/L #	96
38) Bromodichloromethane	9.30	83	7744	0.315	ug/L #	95
39) cis-1,3-Dichloropropene	9.74	75	7902	0.322	ug/L #	79
40) 4-Methyl-2-pentanone	9.88	43	12258	2.117	ug/L #	86
42) Toluene	10.05	91	29097	0.291	ug/L	94
44) trans-1,3-Dichloropropene	10.28	75	3904m	0.248	ug/L	
45) 1,1,2-Trichloroethane	10.46	97	3001	0.305	ug/L #	82
47) Tetrachloroethene	10.53	164	5578	0.331	ug/L	91
48) 2-Hexanone	10.65	43	11381	3.092	ug/L #	96
49) Dibromochloromethane	10.79	129	3209	0.299	ug/L	99
50) 1,2-Dibromoethane	10.90	107	2898	0.339	ug/L #	75
51) Chlorobenzene	11.33	112	18630	0.321	ug/L #	85
52) Ethylbenzene	11.41	91	28389	0.250	ug/L	94
53) m,p-Xylene	11.52	106	10472	0.258	ug/L	86
54) o-Xylene	11.84	106	7500	0.187	ug/L	97
55) Styrene	11.86	104	12514	0.218	ug/L	100
56) Isopropylbenzene	12.14	105	22804	0.202	ug/L	97
58) 1,1,2,2-Tetrachloroethane	12.40	83	4000	0.350	ug/L #	85
59) 1,2,3-Trichloropropane	12.45	75	2854	0.341	ug/L	93
61) Bromoform	12.02	173	2046	0.453	ug/L	88
62) 1,3-Dichlorobenzene	13.18	146	11606	0.282	ug/L	88
63) 1,4-Dichlorobenzene	13.26	146	13052	0.320	ug/L	91
65) 1,2-Dichlorobenzene	13.55	146	12011	0.345	ug/L	89
66) 1,2-Dibromo-3-chloropropan	14.16	75	448m	0.258	ug/L	
67) 1,3,5-Trichlorobenzene	14.31	180	9685	0.291	ug/L	93
68) 1,2,4-trichlorobenzene	14.80	180	6075	0.259	ug/L #	93
69) Naphthalene	15.02	128	5705	0.183	ug/L #	91
70) 1,2,3-Trichlorobenzene	15.20	180	6206	0.298	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VR026636.D
Acq On : 13 Sep 2019 17:20
Operator : SY/MD
Sample : MDL02
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampled :
MDL02

Manual Integrations
APPROVED

MMDadoda
9/16/2019 12:45:01 AM

Quant Time: Sep 14 07:08:51 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 06:49:16 2019
Response via : Initial Calibration

