

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR091418\
 Data File : VR025733.D
 Acq On : 14 Sep 2018 17:01
 Operator : SY/MD
 Sample : J4887-12
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :

Quant Time: Sep 15 03:30:30 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR090718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Sep 15 03:08:36 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	609853	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	516523	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	151161	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.16	65	170957	6.45	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	129.00%
7) Chloroethane-d5	2.63	69	139584	6.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	128.60%
11) 1,1-Dichloroethene-d2	3.63	63	327057	4.51	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	90.20%
20) 2-Butanone-d5	6.60	46	115215	43.05	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.10%
24) Chloroform-d	7.20	84	309176	5.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.00%
26) 1,2-Dichloroethane-d4	7.90	65	110067	5.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.00%
32) Benzene-d6	7.85	84	745585	5.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.80%
36) 1,2-Dichloropropane-d6	8.90	67	202485	5.38	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.60%
41) Toluene-d8	9.97	98	673060	5.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.00%
43) trans-1,3-Dichloropropene-	10.23	79	37924	4.08	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.60%
46) 2-Hexanone-d5	10.59	63	132932	47.88	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.76%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	79700	4.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.80%
64) 1,2-Dichlorobenzene-d4	13.52	152	143669	6.71	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	134.20%#

Target Compounds


					Ovalue
12) 1,1-Dichloroethene	3.65	96	31564	0.79 ug/L	# 1
22) cis-1,2-Dichloroethene	6.67	96	18787	0.44 ug/L	# 89
34) Trichloroethene	8.71	95	506639	11.36 ug/L	# 93
35) Methylcyclohexane	8.89	83	44794	0.65 ug/L	# 20
37) 1,2-Dichloropropane	8.90	63	18619	0.45 ug/L	# 100
66) 1,2-Dibromo-3-chloropropan	14.14	75	284	0.24 ug/L	# 16
69) Naphthalene	15.01	128	10232	0.53 ug/L	# 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR091418\
Data File : VR025733.D
Acq On : 14 Sep 2018 17:01
Operator : SY/MD
Sample : J4887-12
Misc : 25mL/MSVOA R/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :

Quant Time: Sep 15 03:30:30 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR090718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 15 03:08:36 2018
Response via : Initial Calibration

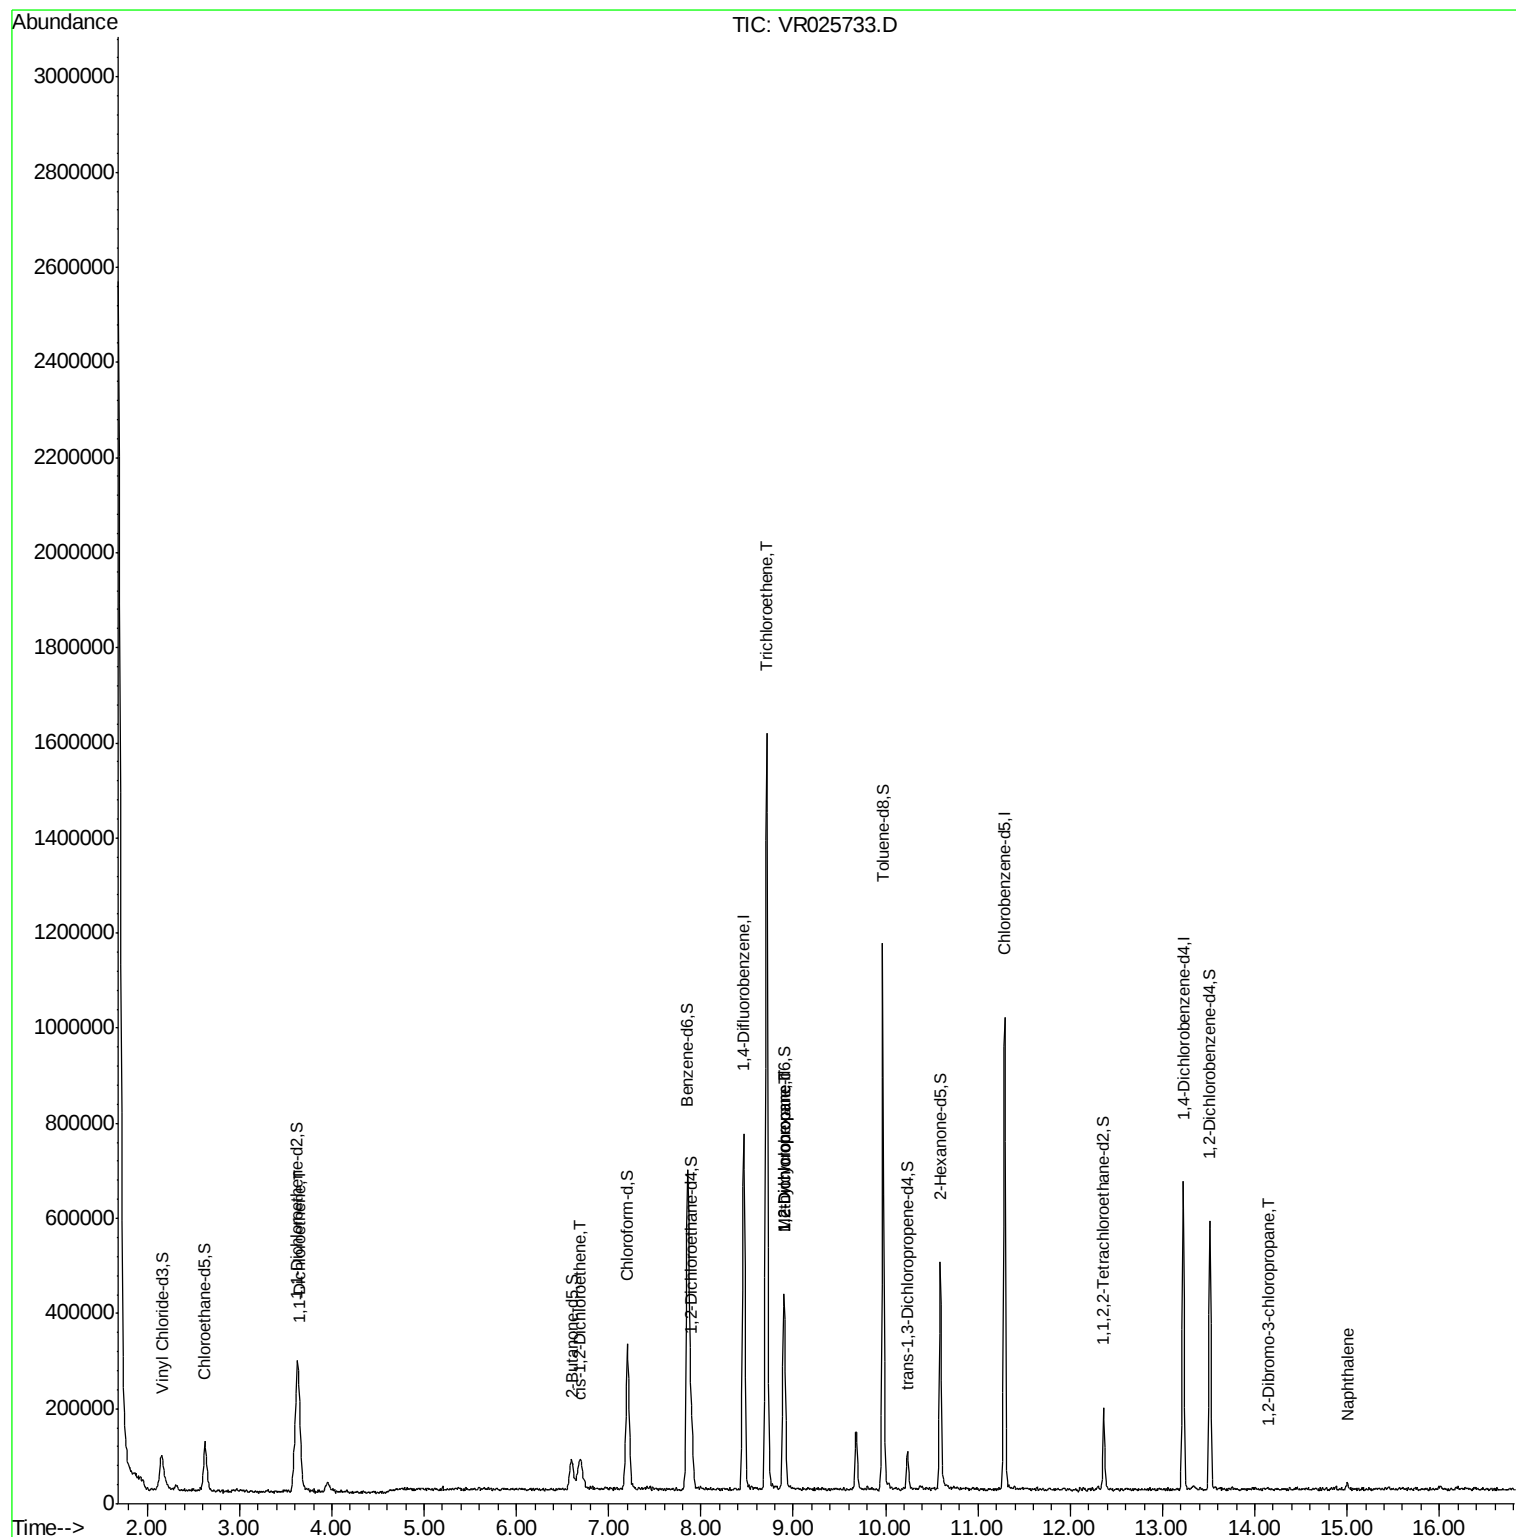

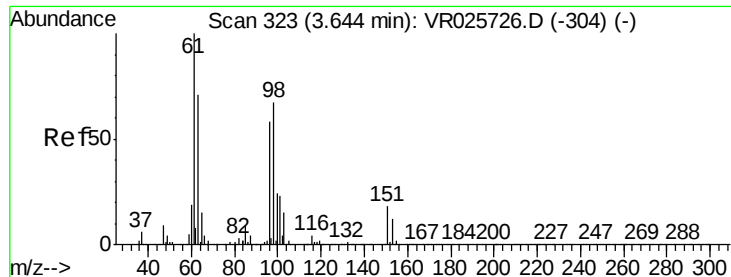

#12

1,1-Dichloroethene

Concen: 0.79 ug/L

RT: 3.65 min Scan# 324





Delta R.T. 0.01 min

Lab File: VR025733.D

Acq: 14 Sep 2018 17:01

Instrument :
MSVOA_R
ClientSampleId :

Tot Ion:	96	Resp:	31564
Ion	Ratio	Lower	Upper
96	100		
61	199.9	128.4	238.4
63	549.3	101.1	187.7#

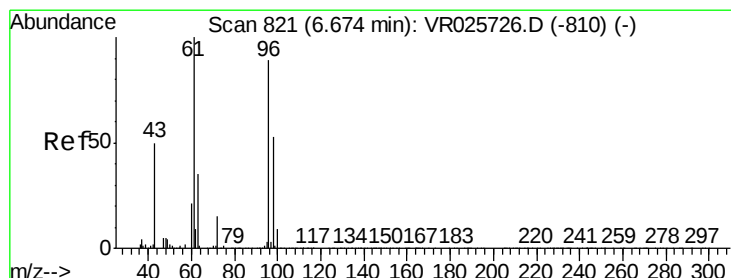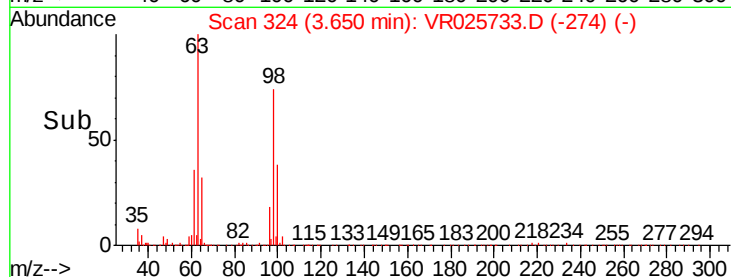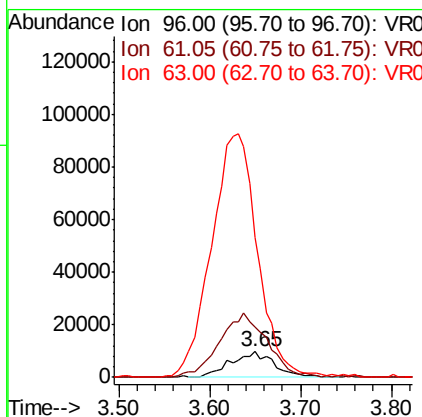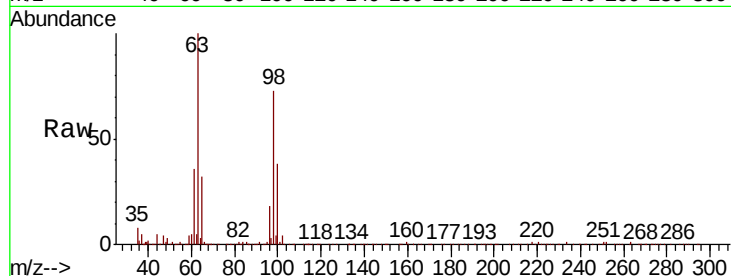

#22

cis-1,2-Dichloroethene

Concen: 0.44 ug/L




RT: 6.67 min Scan# 821


Delta R.T. -0.00 min

Lab File: VR025733.D

Acq: 14 Sep 2018 17:01

Tgt Ion:	96	Resp:	18787
Ion	Ratio	Lower	Upper
96	100		
61	126.6	79.9	148.5
68	0.0	0.2	0.4#


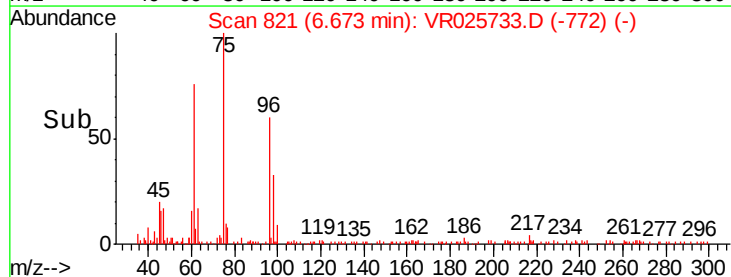
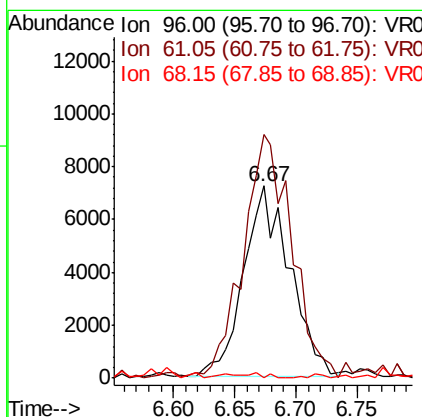
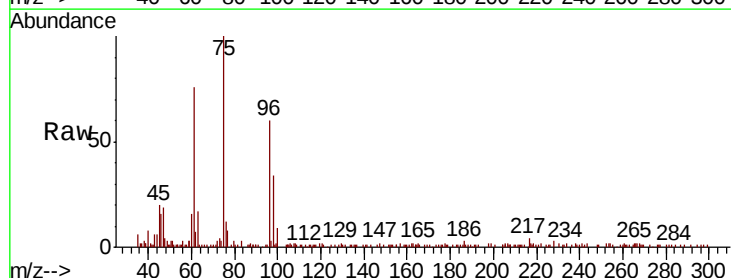


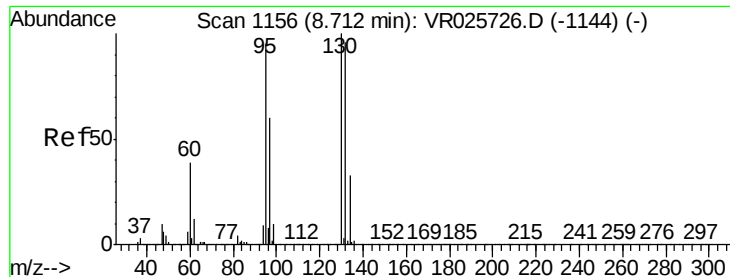

#34
 Trichloroethene
 Concen: 11.36 ug/L
 RT: 8.71 min Scan# 1156
 Delta R.T. -0.00 min
 Lab File: VR025733.D
 Acq: 14 Sep 2018 17:01




Instrument :
 MSVOA_R
 ClientSampleId :


Tot Ion:	95	Resp:	506639
Ion	Ratio	Lower	Upper
95	100		
97	61.9	45.5	84.5
132	93.8	71.0	131.9
130	98.8	74.5	138.3

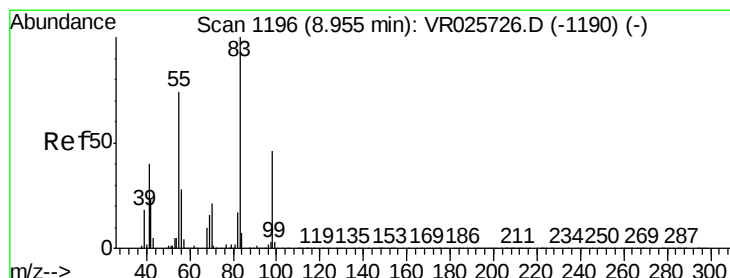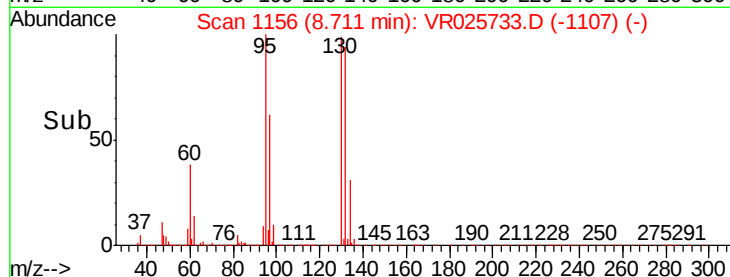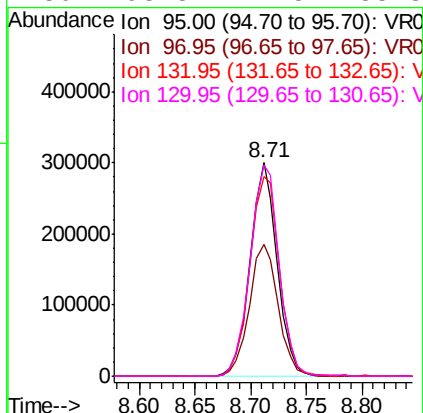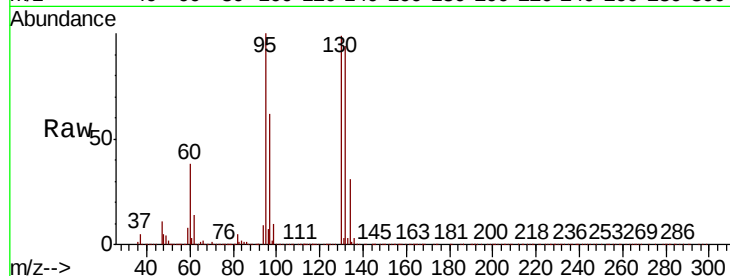

#35
 Methylcyclohexane
 Concen: 0.65 ug/L
 RT: 8.89 min Scan# 1186
 Delta R.T. -0.06 min
 Lab File: VR025733.D
 Acq: 14 Sep 2018 17:01

Tgt Ion:	83	Resp:	44794
Ion	Ratio	Lower	Upper
83	100		
55	0.7	58.9	88.3#
98	0.0	36.9	55.3#


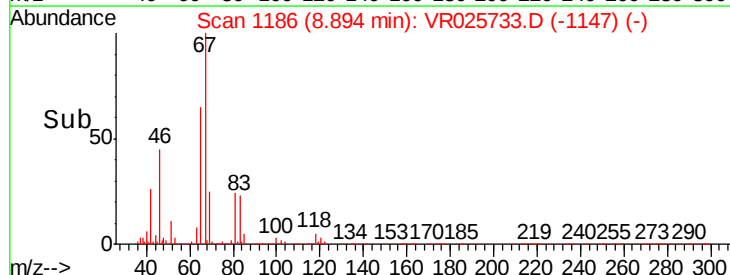
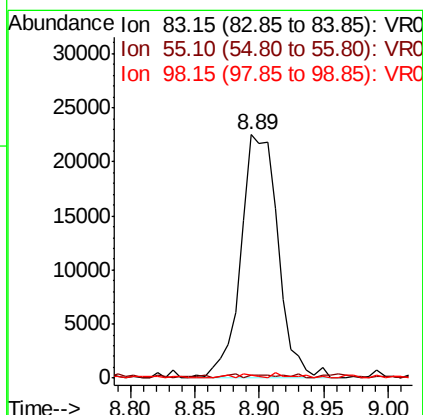
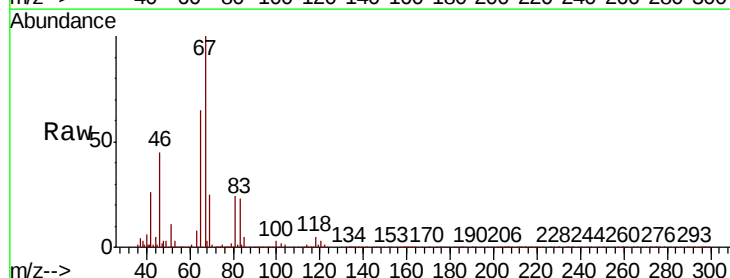


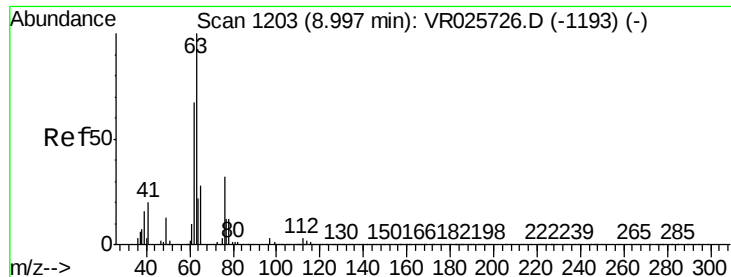

#37
 1,2-Dichloropropane
 Concen: 0.45 ug/L
 RT: 8.90 min Scan# 1187
 Delta R.T. -0.10 min
 Lab File: VR025733.D
 Acq: 14 Sep 2018 17:01




Instrument :
 MSVOA_R
 ClientSampled :


Tot Ion: 63 Resp: 18619
 Ion Ratio Lower Upper
 63 100
 112 3.7 2.9 4.3

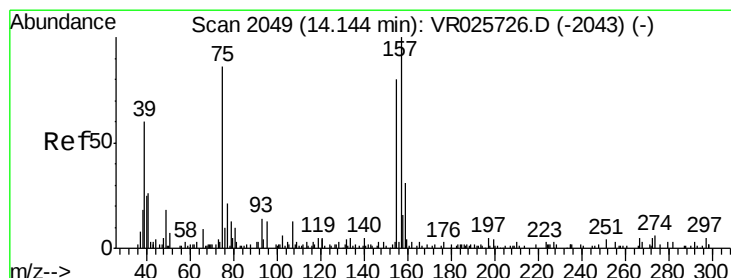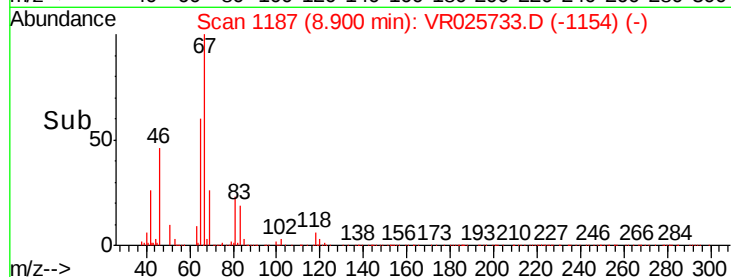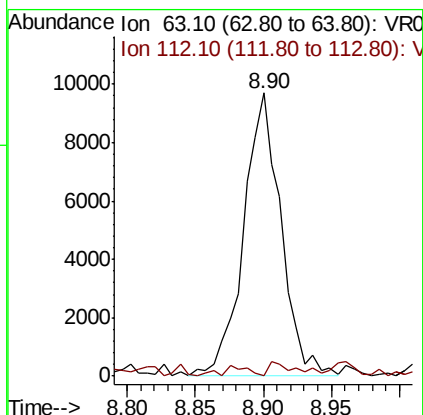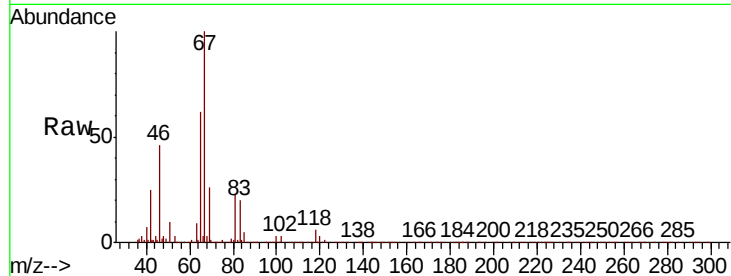

#66
 1,2-Dibromo-3-chloropropane
 Concen: 0.24 ug/L
 RT: 14.14 min Scan# 2048
 Delta R.T. -0.01 min
 Lab File: VR025733.D
 Acq: 14 Sep 2018 17:01

Tgt Ion: 75 Resp: 284
 Ion Ratio Lower Upper
 75 100
 155 0.0 79.3 118.9#
 157 31.9 81.4 122.2#

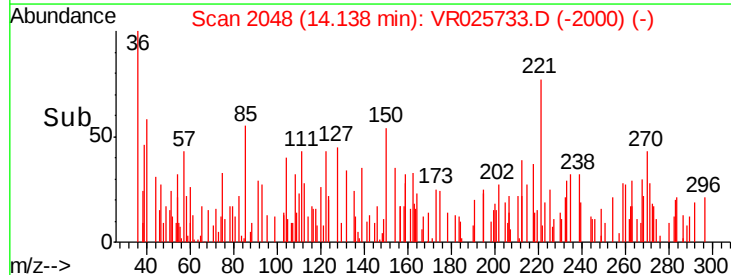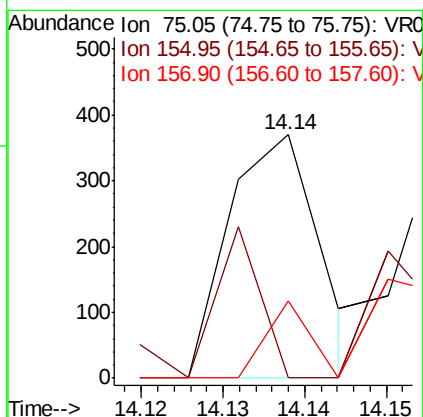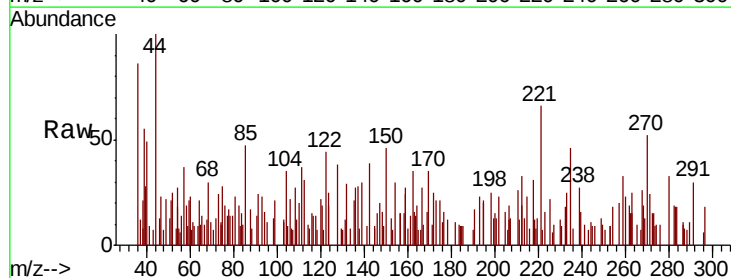

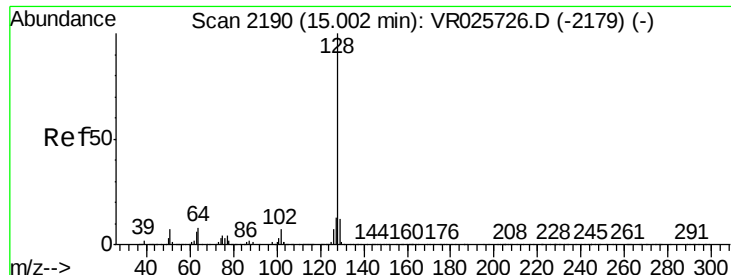

#69

Naphthalene

Concen: 0.53 ug/L

RT: 15.01 min Scan# 2191

Delta R.T. 0.01 min


Lab File: VR025733.D

Acq: 14 Sep 2018 17:01

Instrument :

MSVOA_R

ClientSampleId :

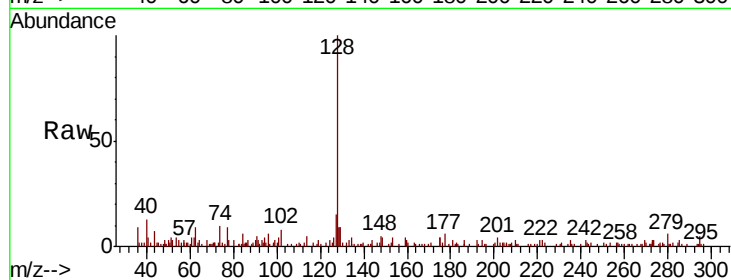

Tot Ion:	128	Resp:	10232
Ion	Ratio	Lower	Upper
128	100		
127	18.4	10.3	15.5#
129	15.8	9.0	13.6#

