

#5

Vinyl chloride

Concen: 0.912 ug/L

RT: 2.16 min Scan# 79

Delta R.T. -0.01 min

Lab File: VR025770.D

Acq: 20 Sep 2018 10:54

Instrument :

MSVOA_R


ClientSampleId :

Tgt Ion: 62 Resp: 34507

Ion Ratio Lower Upper

62 100

64 29.6 20.9 38.9

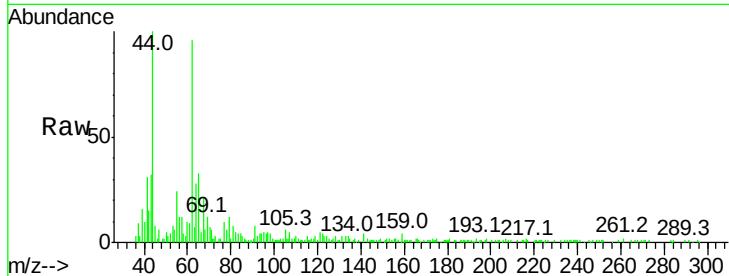

Abundance Ion 62.00 (61.70 to 62.70): VR0

Ion 64.10 (63.80 to 64.80): VR0

15000

10000



5000

0

2.16

2.00 2.10 2.20 2.30

Time-->

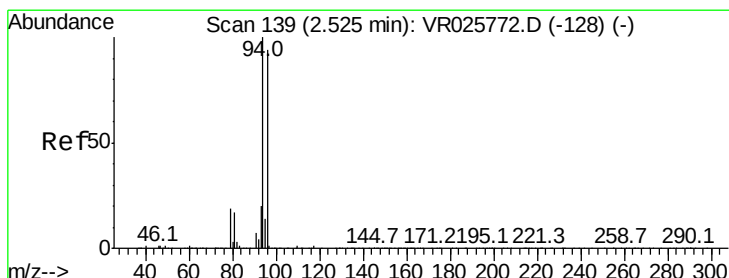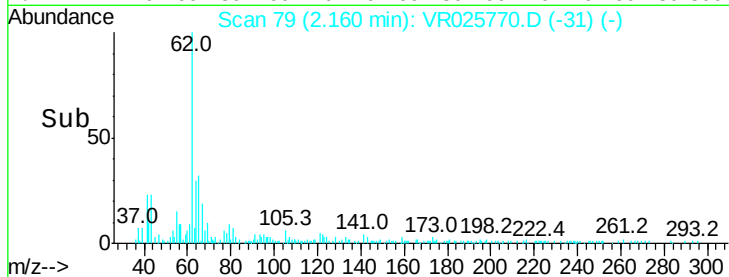

#6

Bromomethane

Concen: 0.685 ug/L

RT: 2.52 min Scan# 138

Delta R.T. -0.01 min

Lab File: VR025770.D


Acq: 20 Sep 2018 10:54

Tgt Ion: 94 Resp: 18555

Ion Ratio Lower Upper

94 100

96 80.0 66.1 122.7

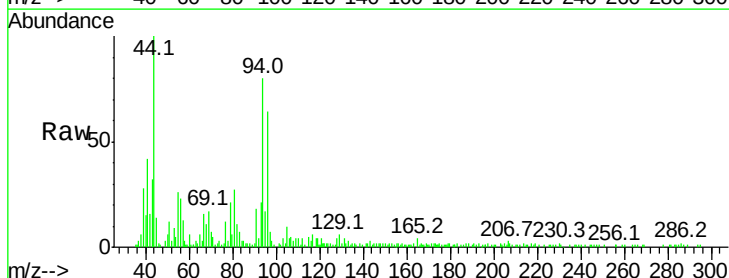

Abundance Ion 94.00 (93.70 to 94.70): VR0

Ion 96.00 (95.70 to 96.70): VR0

10000

8000

6000

4000

2000

0

2.52

2.45 2.50 2.55 2.60

Time-->

