

#8

Chloroethane

Concen: 0.870 ug/L

RT: 2.66 min Scan# 161

Delta R.T. -0.00 min

Lab File: VR025770.D

Acq: 20 Sep 2018 10:54

Instrument :

MSVOA_R


ClientSampleId :

Tgt Ion: 64 Resp: 19336

Ion Ratio Lower Upper




64 100

66 36.4 21.9 40.7

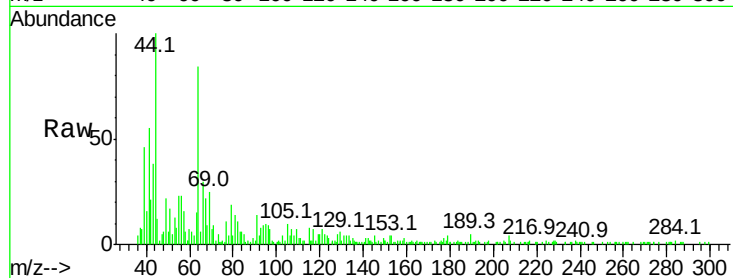

Abundance Ion 64.10 (63.80 to 64.80): VR0

Ion 66.05 (65.75 to 66.75): VR0

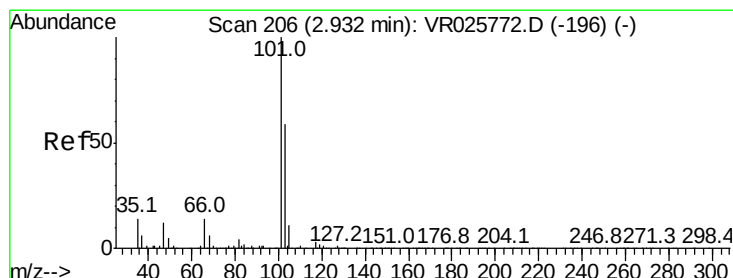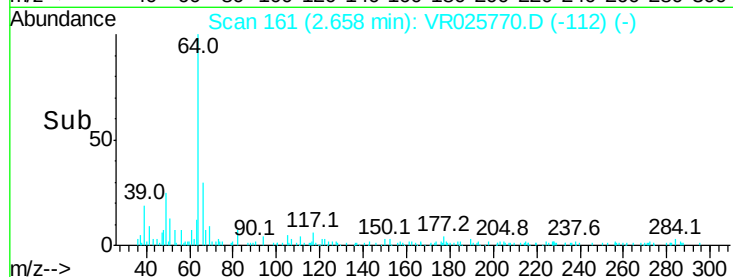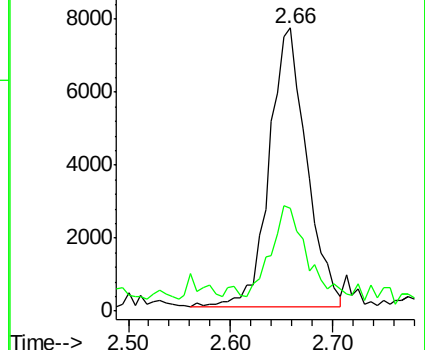

#9

Trichlorofluoromethane

Concen: 0.201 ug/L

RT: 2.93 min Scan# 205

Delta R.T. -0.01 min

Lab File: VR025770.D


Acq: 20 Sep 2018 10:54

Tgt Ion: 101 Resp: 14021

Ion Ratio Lower Upper

101 100

103 100.6 20.2 30.2#

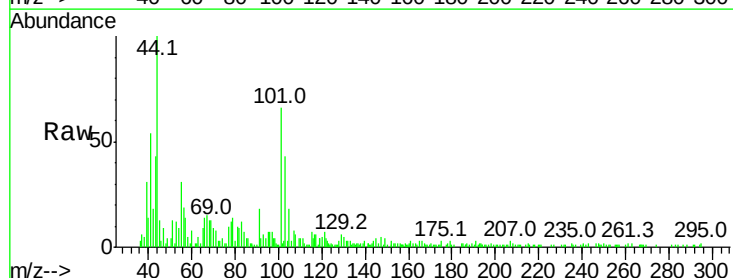

Abundance Ion 101.00 (100.70 to 101.70): V

Ion 103.00 (102.70 to 103.70): V

