

#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.619 ug/L

RT: 3.68 min Scan# 329





Delta R.T. 0.01 min

Lab File: VR025770.D

Acq: 20 Sep 2018 10:54

Instrument :
MSVOA_R
ClientSampleId :

Tgt Ion:	101	Resp:	23286
Ion	Ratio	Lower	Upper
101	100		
85	50.5	37.6	56.4
151	84.1	60.9	91.3

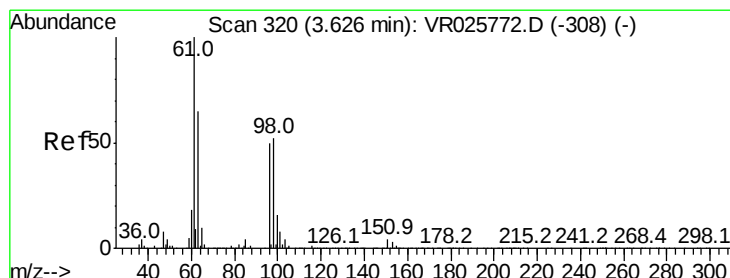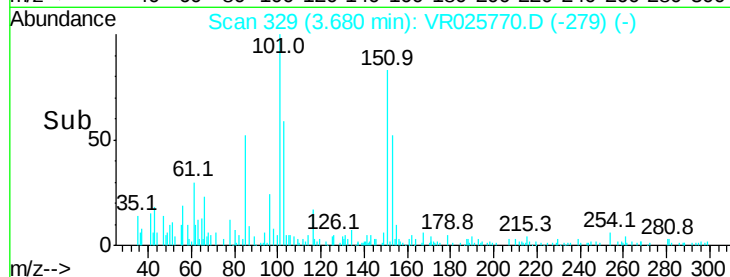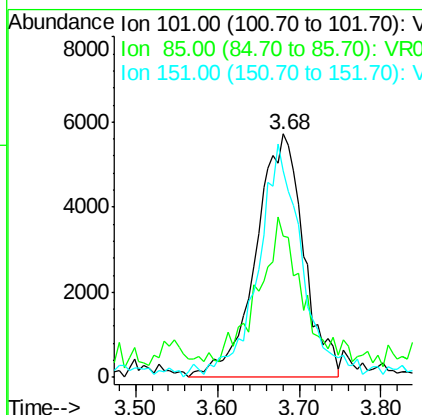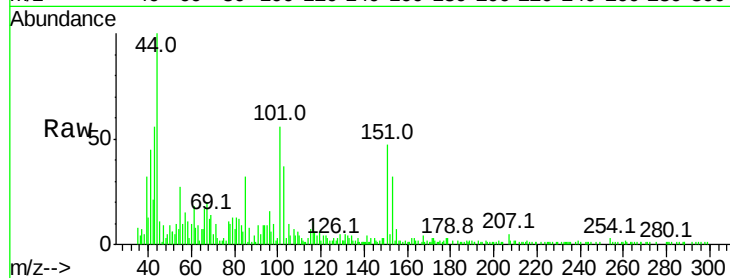

#12

1,1-Dichloroethene

Concen: 0.645 ug/L

RT: 3.64 min Scan# 322

Delta R.T. 0.01 min

Lab File: VR025770.D

Acq: 20 Sep 2018 10:54

Tgt Ion:	96	Resp:	25617
Ion	Ratio	Lower	Upper
96	100		
61	164.1	138.7	257.7
63	88.9	90.9	168.7#

