
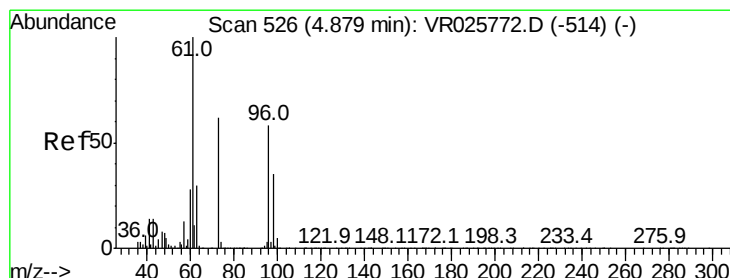
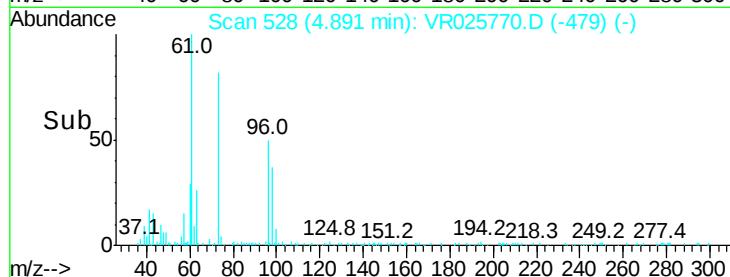
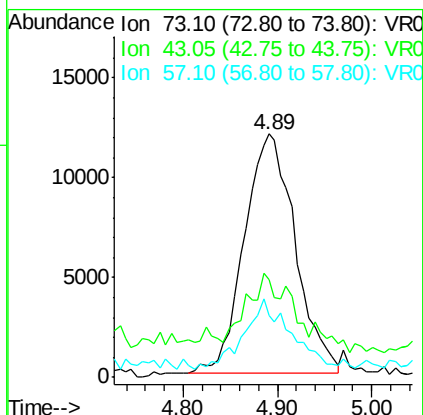


#17

Methyl tert-butyl Ether
 Concen: 0.928 ug/L
 RT: 4.89 min Scan# 528
 Delta R.T. -0.00 min
 Lab File: VR025770.D
 Acq: 20 Sep 2018 10:54

Instrument :
 MSVOA_R
 ClientSampleId :

Tgt Ion:	73	Resp:	45319
Ion	Ratio	Lower	Upper
73	100		
43	22.1	20.4	30.6
57	26.5	17.8	26.6

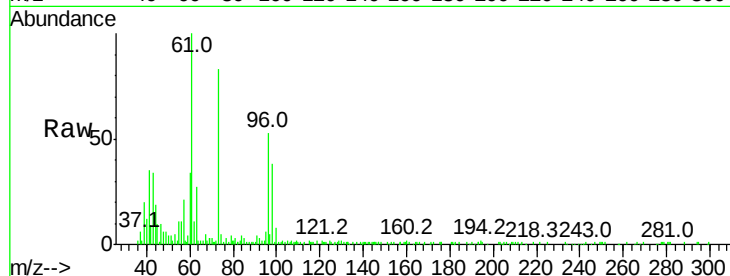

#18

trans-1,2-Dichloroethene
 Concen: 0.659 ug/L
 RT: 4.88 min Scan# 526
 Delta R.T. -0.00 min
 Lab File: VR025770.D
 Acq: 20 Sep 2018 10:54

Tgt Ion:	96	Resp:	31953
Ion	Ratio	Lower	Upper
96	100		
61	152.4	121.4	225.6
98	54.6	42.7	79.3

