





#29
 1,1,1-Trichloroethane
 Concen: 1.135 ug/L
 RT: 7.43 min Scan# 945
 Delta R.T. -0.00 min
 Lab File: VR025770.D
 Acq: 20 Sep 2018 10:54

Instrument :
 MSVOA_R
 ClientSampled :

Tgt Ion: 97 Resp: 54808
 Ion Ratio Lower Upper
 97 100
 99 65.2 51.0 76.6
 61 53.9 40.4 60.6

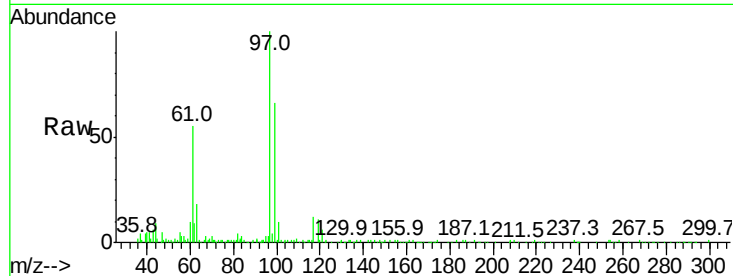


Abundance Ion 96.95 (96.65 to 97.65): VR0
 Ion 99.05 (98.75 to 99.75): VR0
 Ion 61.05 (60.75 to 61.75): VR0

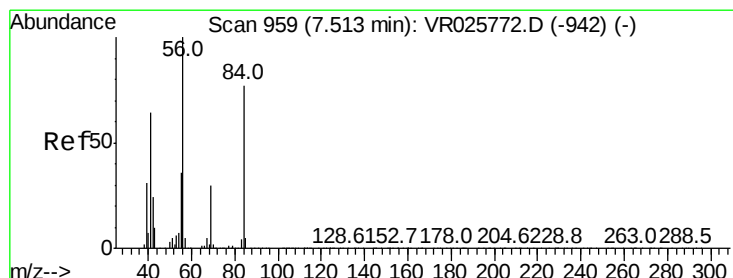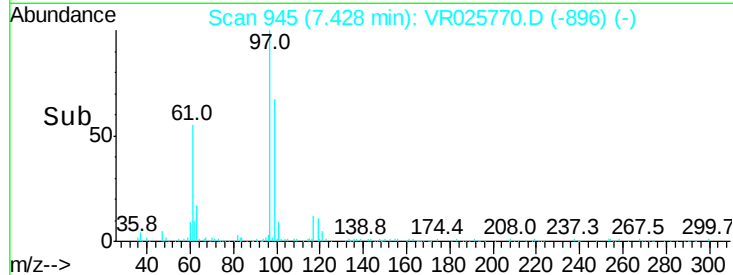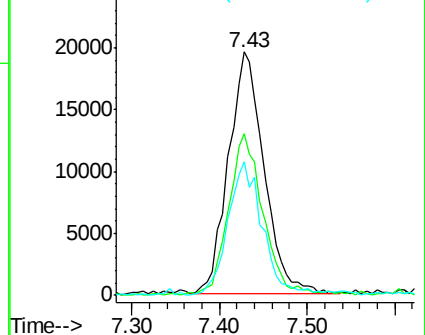

#30
 Cyclohexane
 Concen: 1.084 ug/L
 RT: 7.51 min Scan# 959
 Delta R.T. -0.00 min
 Lab File: VR025770.D
 Acq: 20 Sep 2018 10:54

Tgt Ion: 56 Resp: 62918
 Ion Ratio Lower Upper
 56 100
 69 33.0 24.0 36.0
 84 76.6 60.2 90.4

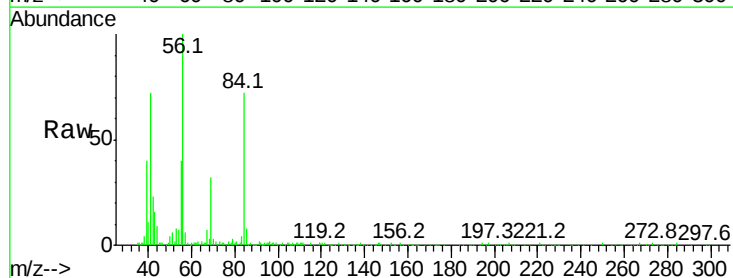

Abundance Ion 56.10 (55.80 to 56.80): VR0
 Ion 69.15 (68.85 to 69.85): VR0
 Ion 84.15 (83.85 to 84.85): VR0

