

#34

Trichloroethene

Concen: 0.832 ug/L

RT: 8.71 min Scan# 1155

Delta R.T. -0.01 min

Lab File: VR025770.D

Acq: 20 Sep 2018 10:54

Instrument :

MSVOA_R

ClientSampleId :

Tgt Ion: 95 Resp: 34833


Ion Ratio Lower Upper

95 100

97 68.4 46.2 85.8

132 87.4 56.0 104.0

130 80.0 59.6 110.8



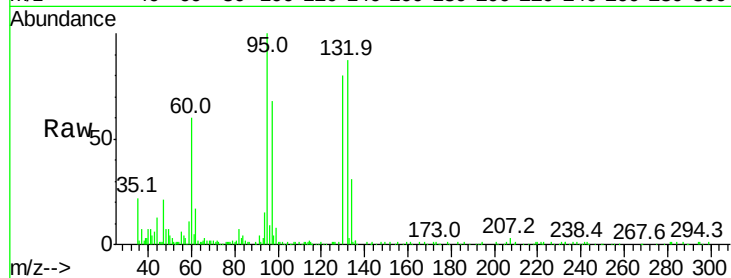


Abundance Ion 95.00 (94.70 to 95.70): VR0

Ion 96.95 (96.65 to 97.65): VR0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

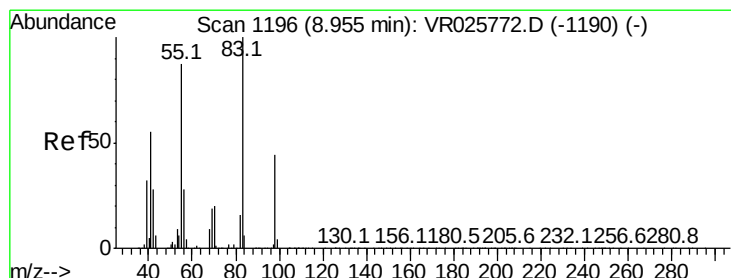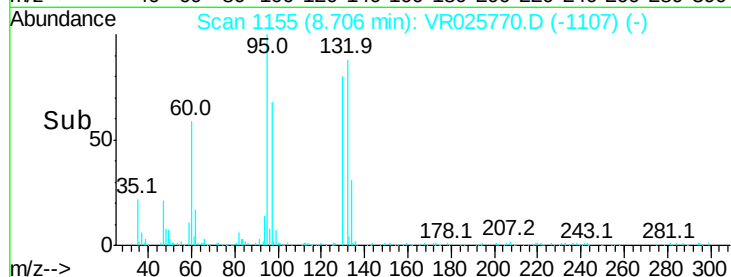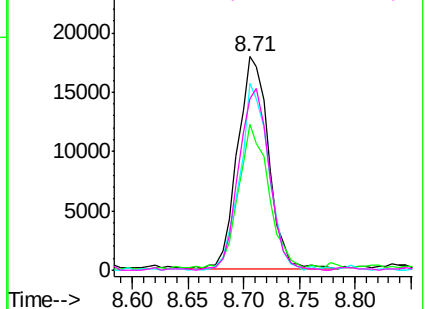

#35

Methylcyclohexane

Concen: 0.913 ug/L

RT: 8.95 min Scan# 1195

Delta R.T. -0.01 min

Lab File: VR025770.D

Acq: 20 Sep 2018 10:54


Tgt Ion: 83 Resp: 59000

Ion Ratio Lower Upper

83 100

55 93.7 70.3 105.5

98 45.9 34.4 51.6

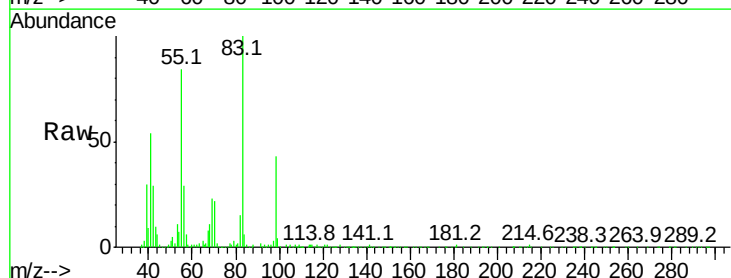

Abundance Ion 83.15 (82.85 to 83.85): VR0

Ion 55.10 (54.80 to 55.80): VR0

Ion 98.15 (97.85 to 98.85): VR0

