

#37

1,2-Dichloropropane

Concen: 0.724 ug/L

RT: 9.00 min Scan# 1203

Delta R.T. 0.01 min

Lab File: VR025770.D

Acq: 20 Sep 2018 10:54

Instrument :

MSVOA\_R


ClientSampleId :

Tgt Ion: 63 Resp: 28180

Ion Ratio Lower Upper




63 100

112 3.9 3.0 4.6

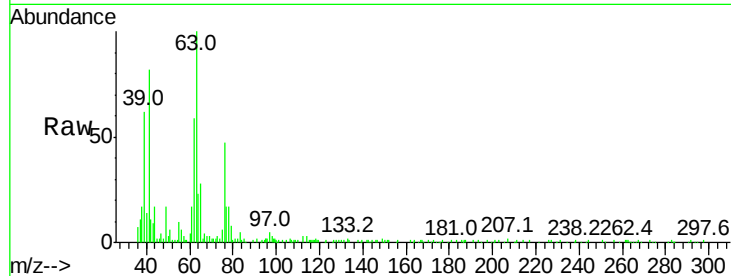

Abundance Ion 63.10 (62.80 to 63.80): VR0

Ion 112.10 (111.80 to 112.80): V

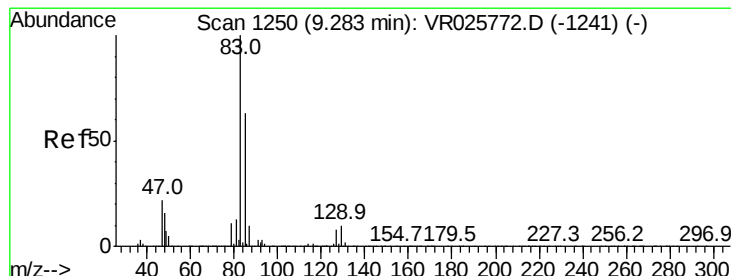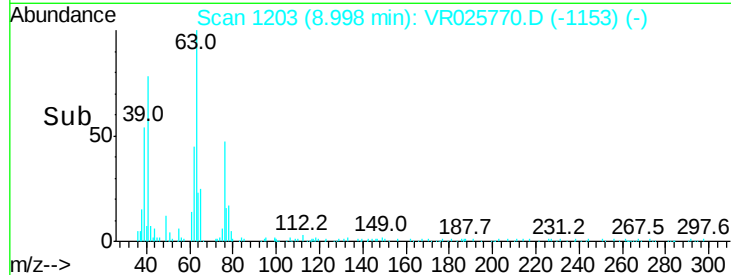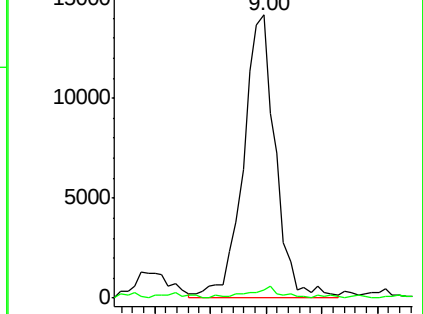

#38

Bromodichloromethane

Concen: 0.964 ug/L

RT: 9.28 min Scan# 1249

Delta R.T. -0.01 min

Lab File: VR025770.D

Acq: 20 Sep 2018 10:54


Tgt Ion: 83 Resp: 33697

Ion Ratio Lower Upper

83 100

85 60.8 44.2 82.0

127 7.1 6.0 9.0

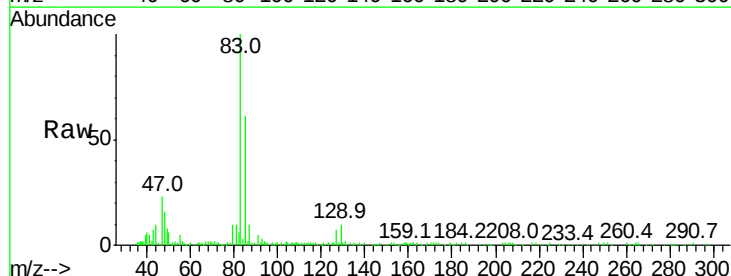

Abundance Ion 82.95 (82.65 to 83.65): VR0

Ion 85.00 (84.70 to 85.70): VR0

Ion 126.90 (126.60 to 127.60): V

