
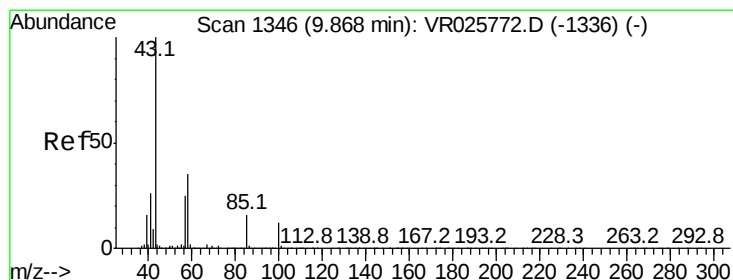
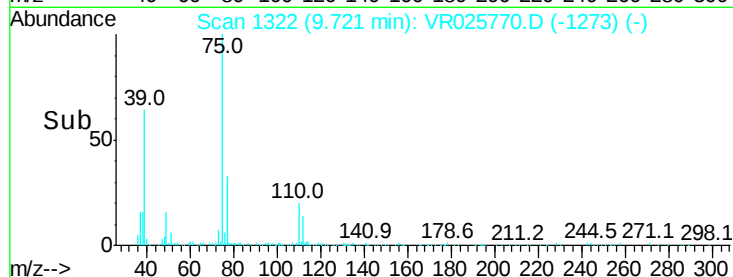
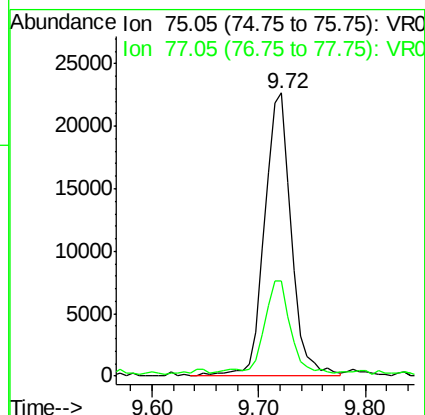


#39
 cis-1,3-Dichloropropene
 Concen: 0.990 ug/L
 RT: 9.72 min Scan# 1322
 Delta R.T. -0.00 min
 Lab File: VR025770.D
 Acq: 20 Sep 2018 10:54

Instrument :
 MSVOA_R
 ClientSampled :

Tgt Ion: 75 Resp: 39403
 Ion Ratio Lower Upper
 75 100
 77 33.6 21.2 39.4

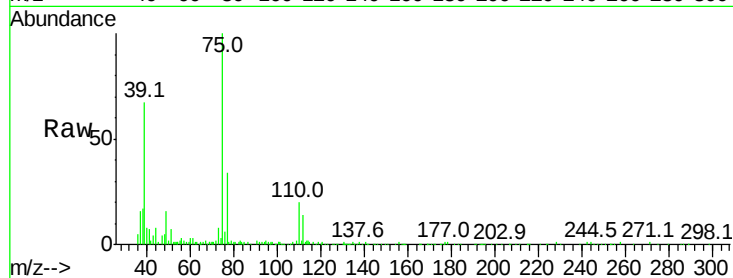

#40
 4-Methyl-2-pentanone
 Concen: 9.886 ug/L
 RT: 9.87 min Scan# 1346
 Delta R.T. -0.00 min
 Lab File: VR025770.D
 Acq: 20 Sep 2018 10:54

Tgt Ion: 43 Resp: 95151
 Ion Ratio Lower Upper
 43 100
 58 35.9 28.3 42.5
 100 11.7 9.3 13.9

