

#42

Toluene

Concen: 0.716 ug/L

RT: 10.03 min Scan# 1373

Delta R.T. -0.00 min

Lab File: VR025770.D

Acq: 20 Sep 2018 10:54

Instrument :

MSVOA_R


ClientSampleId :

Tgt Ion: 91 Resp: 126570

Ion Ratio Lower Upper




91 100

92 61.2 41.1 76.3

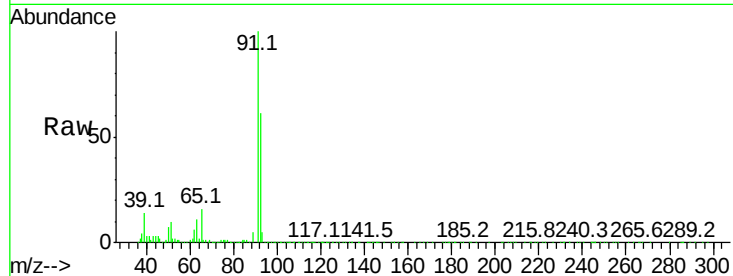

Abundance Ion 91.15 (90.85 to 91.85): VR0

Ion 92.15 (91.85 to 92.85): VR0

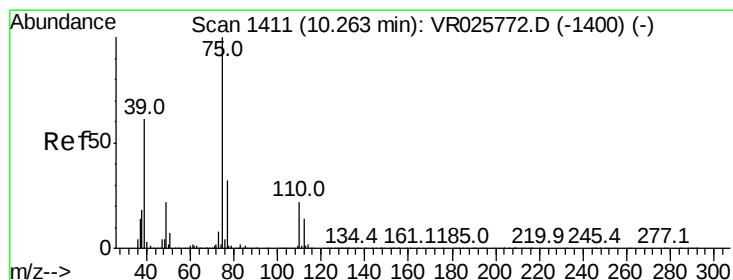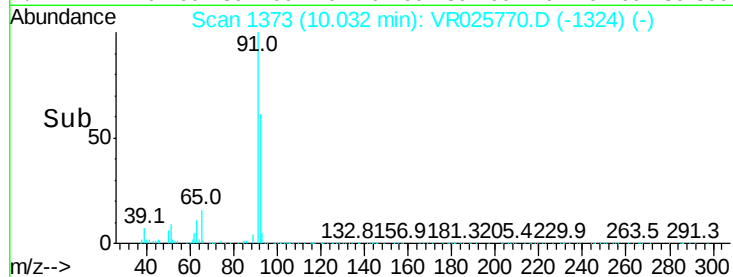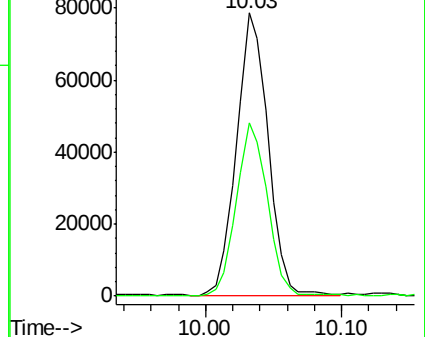

#44

trans-1,3-Dichloropropene

Concen: 1.013 ug/L

RT: 10.26 min Scan# 1411

Delta R.T. -0.00 min

Lab File: VR025770.D


Acq: 20 Sep 2018 10:54

Tgt Ion: 75 Resp: 28374

Ion Ratio Lower Upper

75 100

77 30.7 22.6 42.0

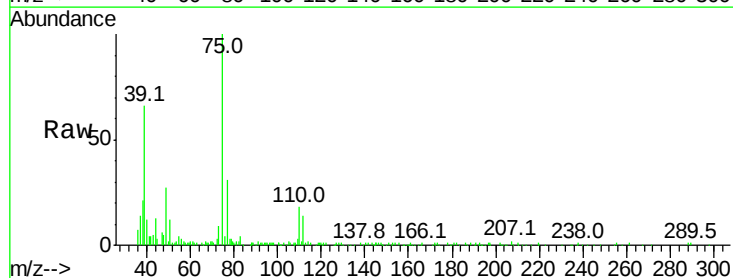

Abundance Ion 75.05 (74.75 to 75.75): VR0

Ion 77.05 (76.75 to 77.75): VR0

