

#45

1,1,2-Trichloroethane

Concen: 0.647 ug/L

RT: 10.45 min Scan# 1441

Delta R.T. -0.00 min

Lab File: VR025770.D

Acq: 20 Sep 2018 10:54

Instrument :

MSVOA_R

ClientSampleId :

Tgt Ion: 97 Resp: 11808


Ion Ratio Lower Upper

97 100

99 65.4 41.2 76.4

83 92.7 61.3 113.9

85 59.3 38.9 72.2



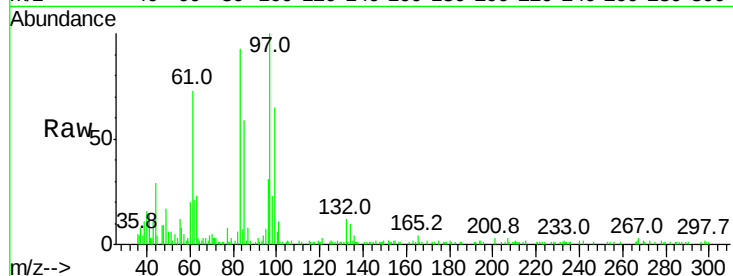


Abundance Ion 96.95 (96.65 to 97.65): VR0

Ion 99.05 (98.75 to 99.75): VR0

Ion 82.95 (82.65 to 83.65): VR0

Ion 85.00 (84.70 to 85.70): VR0

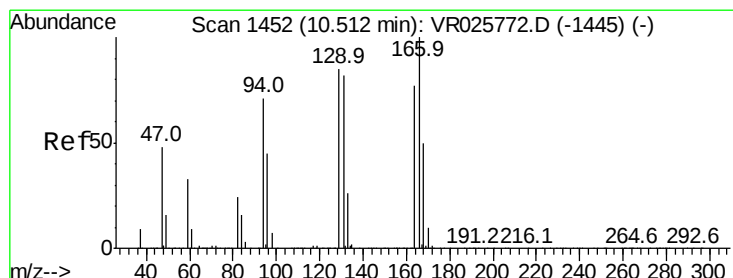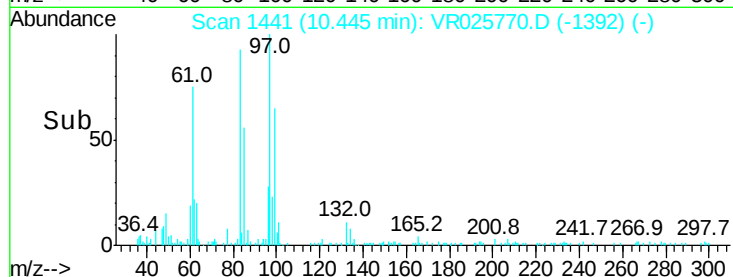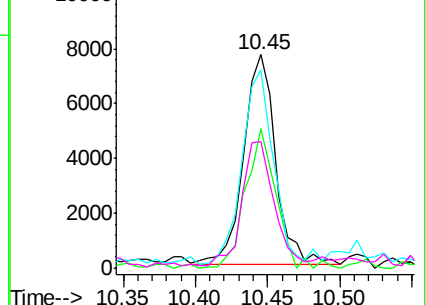

#47

Tetrachloroethene

Concen: 0.608 ug/L

RT: 10.51 min Scan# 1452

Delta R.T. -0.00 min

Lab File: VR025770.D

Acq: 20 Sep 2018 10:54

Tgt Ion: 164 Resp: 20851


Ion Ratio Lower Upper

164 100

129 115.1 77.5 143.9

131 114.0 74.3 138.1

166 139.3 91.1 169.1

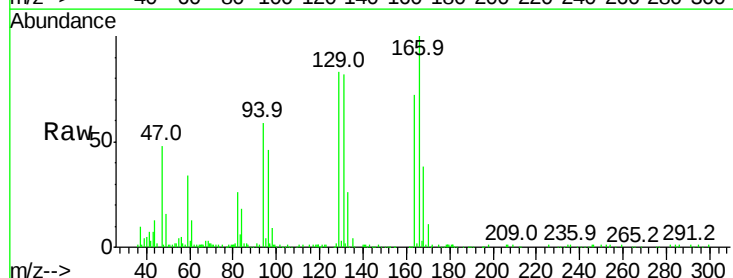

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

