
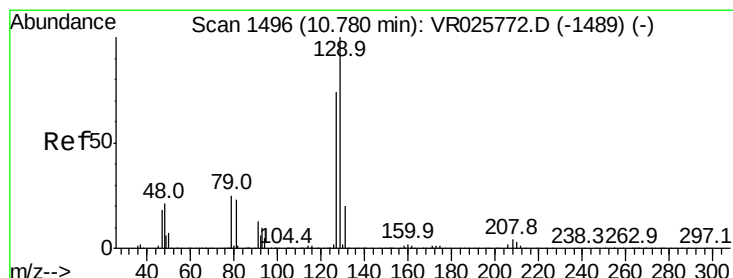
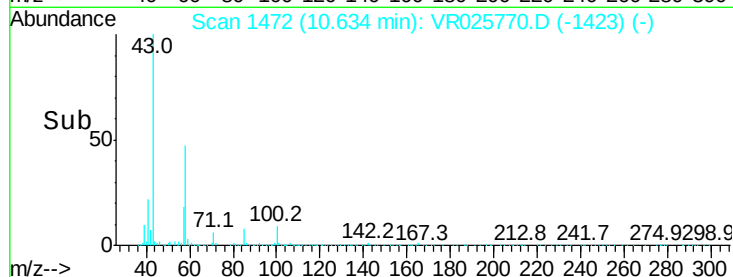
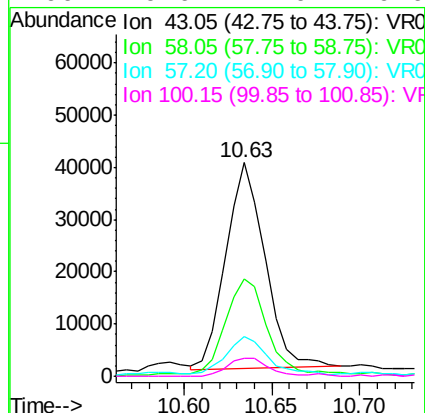


#48
2-Hexanone
Concen: 9.057 ug/L
RT: 10.63 min Scan# 1472
Delta R.T. -0.00 min
Lab File: VR025770.D
Acq: 20 Sep 2018 10:54

Instrument :
MSVOA_R
ClientSampleId :

Tgt Ion:	43	Resp:	61136
Ion	Ratio	Lower	Upper
43	100		
58	54.4	39.9	59.9
57	19.9	14.3	21.5
100	9.6	7.0	10.6

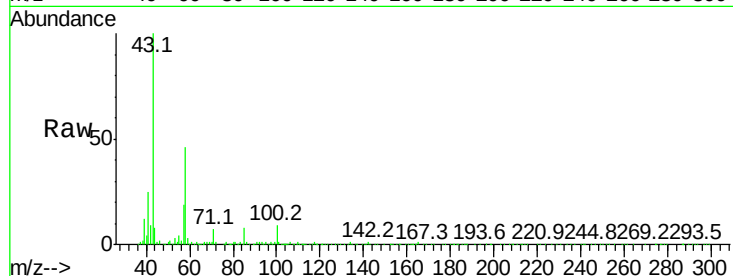

#49
Dibromochloromethane
Concen: 0.750 ug/L
RT: 10.79 min Scan# 1497
Delta R.T. 0.01 min
Lab File: VR025770.D
Acq: 20 Sep 2018 10:54

Tgt Ion:	129	Resp:	14571
Ion	Ratio	Lower	Upper
129	100		
127	78.7	51.9	96.5

