

#52

Ethylbenzene

Concen: 0.835 ug/L

RT: 11.39 min Scan# 1596

Delta R.T. -0.01 min

Lab File: VR025770.D

Acq: 20 Sep 2018 10:54

Instrument :

MSVOA_R





ClientSampleId :

Tgt Ion: 91 Resp: 159053

Ion Ratio Lower Upper

91 100

106 27.6 21.4 39.8

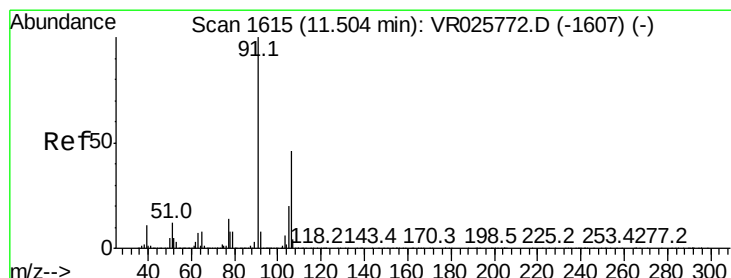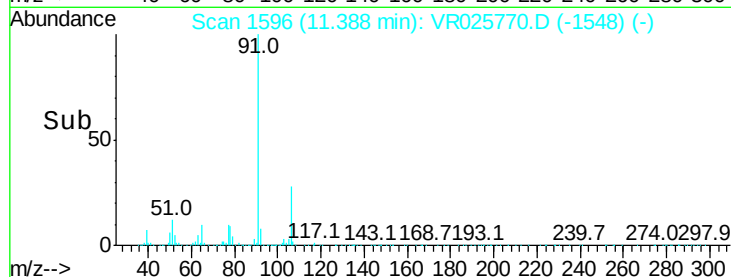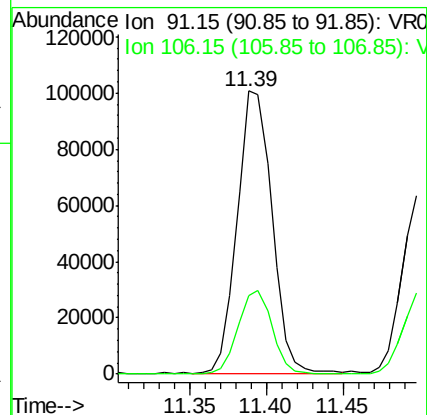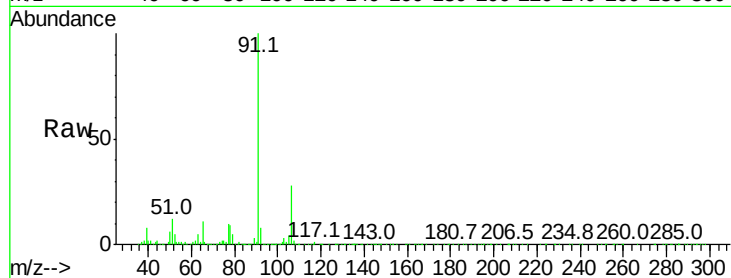

#53

m,p-Xylene

Concen: 0.732 ug/L

RT: 11.50 min Scan# 1615

Delta R.T. -0.00 min

Lab File: VR025770.D

Acq: 20 Sep 2018 10:54

Tgt Ion: 106 Resp: 56102

Ion Ratio Lower Upper

106 100

91 221.2 154.3 286.5

