

#59

1,2,3-Trichloropropane

Concen: 0.852 ug/L

RT: 12.43 min Scan# 1768

Delta R.T. -0.00 min

Lab File: VR025770.D

Acq: 20 Sep 2018 10:54

Instrument :

MSVOA_R





ClientSampleId :

Tgt Ion: 75 Resp: 10185

Ion Ratio Lower Upper

75 100

77 35.4 25.6 38.4

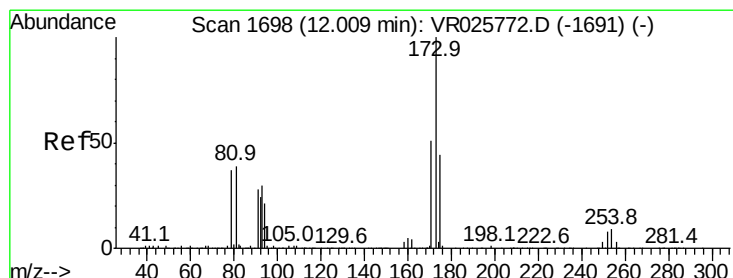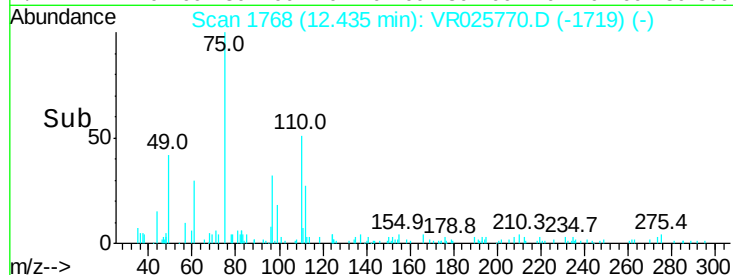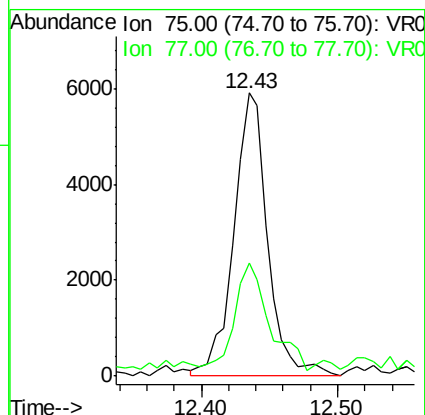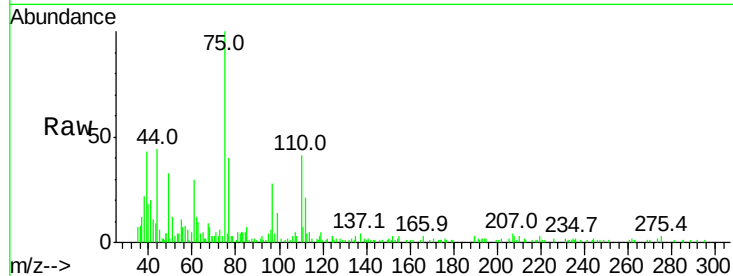

#61

Bromoform

Concen: 0.725 ug/L

RT: 12.00 min Scan# 1697

Delta R.T. -0.01 min

Lab File: VR025770.D

Acq: 20 Sep 2018 10:54

Tgt Ion: 173 Resp: 5511

Ion Ratio Lower Upper

173 100

175 57.9 39.9 59.9

254 15.2 6.6 9.8#

