

#62

1,3-Dichlorobenzene

Concen: 0.788 ug/L

RT: 13.16 min Scan# 1888

Delta R.T. -0.00 min

Lab File: VR025770.D


Acq: 20 Sep 2018 10:54

Instrument :

MSVOA_R

ClientSampleId :




Tgt Ion:	146	Resp:	43725
Ion Ratio	Lower	Upper	
146	100		
111	44.8	32.1	59.5
148	61.4	44.3	82.3

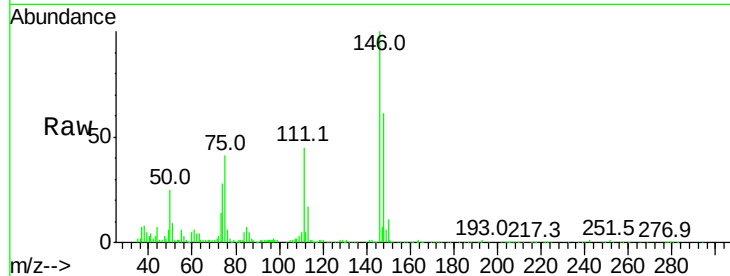

Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

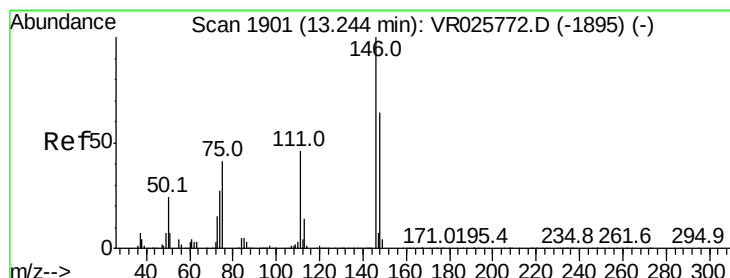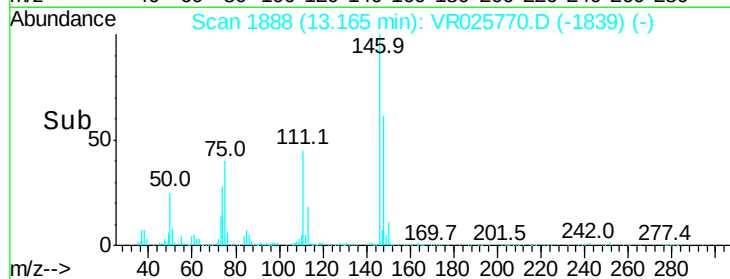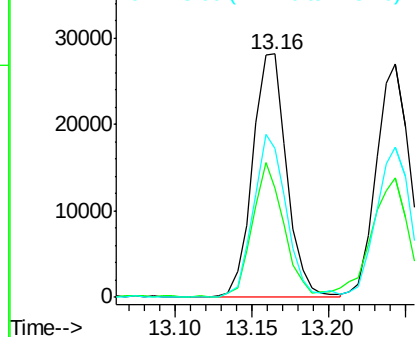

#63

1,4-Dichlorobenzene

Concen: 0.651 ug/L


RT: 13.24 min Scan# 1901

Delta R.T. -0.00 min

Lab File: VR025770.D

Acq: 20 Sep 2018 10:54

Tgt Ion:	146	Resp:	41111
Ion Ratio	Lower	Upper	
146	100		
111	51.0	32.3	60.1
148	64.5	44.6	82.8

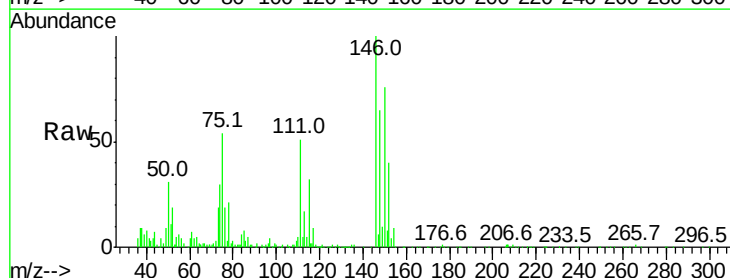

Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

