
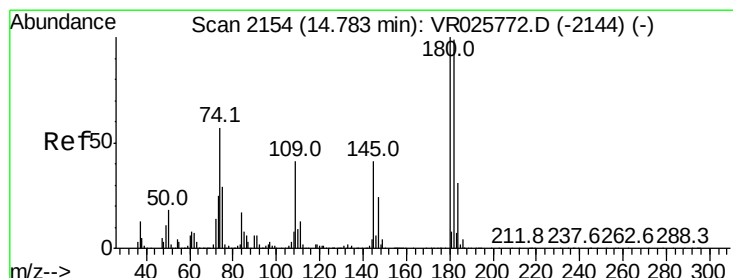
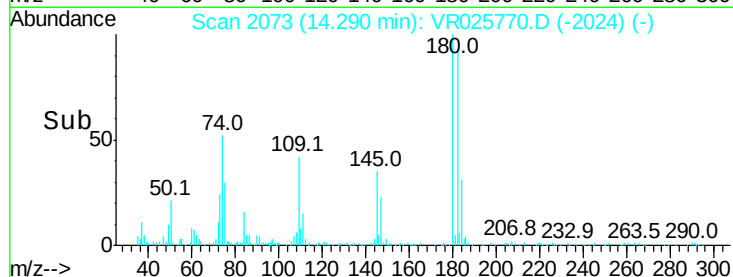
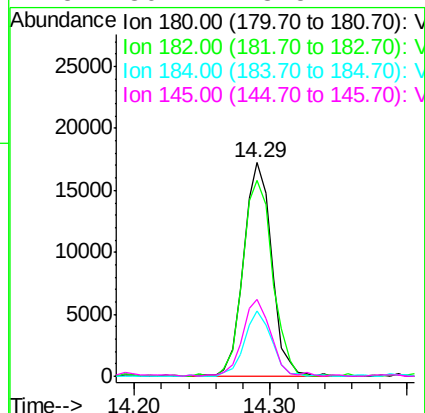


#67
 1,3,5-Trichlorobenzene
 Concen: 0.754 ug/L
 RT: 14.29 min Scan# 2073
 Delta R.T. -0.00 min
 Lab File: VR025770.D
 Acq: 20 Sep 2018 10:54

Instrument :
 MSVOA_R
 ClientSampled :

Tgt Ion:	180	Resp:	24883
Ion Ratio	Lower	Upper	
180	100		
182	97.1	75.7	113.5
184	30.0	24.8	37.2
145	36.4	28.5	42.7

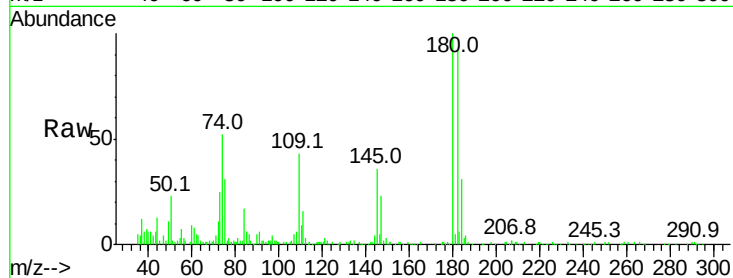

#68
 1,2,4-trichlorobenzene
 Concen: 0.835 ug/L
 RT: 14.78 min Scan# 2154
 Delta R.T. -0.00 min
 Lab File: VR025770.D
 Acq: 20 Sep 2018 10:54

Tgt Ion:	180	Resp:	16906
Ion Ratio	Lower	Upper	
180	100		
182	92.8	76.2	114.2
145	36.4	30.2	45.2

