

#69

Naphthalene

Concen: 1.015 ug/L

RT: 15.00 min Scan# 2190

Delta R.T. -0.00 min

Lab File: VR025770.D





Acq: 20 Sep 2018 10:54

Instrument :

MSVOA_R

ClientSampled :

Tgt Ion:	128	Resp:	22987
Ion	Ratio	Lower	Upper
128	100		
127	16.6	10.3	15.5#
129	9.8	9.1	13.7

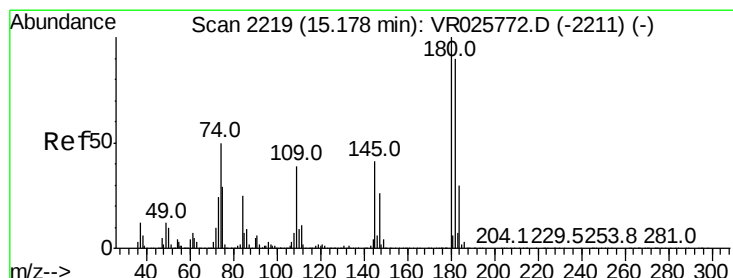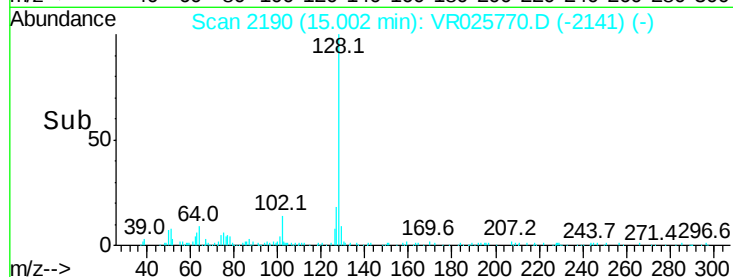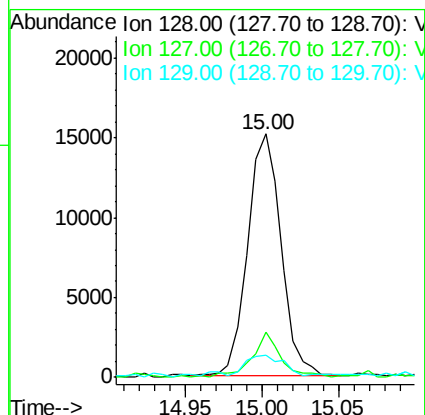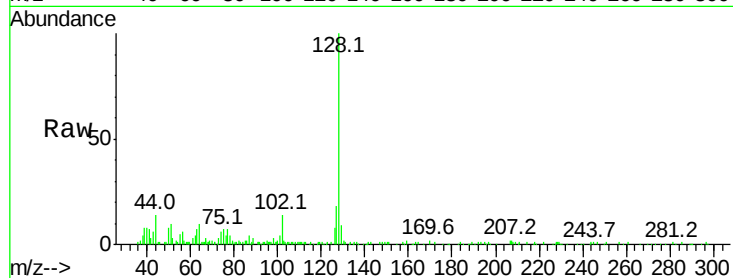

#70

1,2,3-Trichlorobenzene

Concen: 0.729 ug/L

RT: 15.18 min Scan# 2219

Delta R.T. -0.00 min

Lab File: VR025770.D

Acq: 20 Sep 2018 10:54

Tgt Ion:	180	Resp:	11681
Ion	Ratio	Lower	Upper
180	100		
182	99.8	75.7	113.5
145	39.4	31.8	47.8

