

#5

Vinyl chloride

Concen: 1.682 ug/L

RT: 2.16 min Scan# 79

Delta R.T. -0.01 min

Lab File: VR025771.D

Acq: 20 Sep 2018 11:28

Instrument :

MSVOA_R





ClientSampleId :

Tgt Ion: 62 Resp: 60396

Ion Ratio Lower Upper

62 100

64 33.0 20.9 38.9

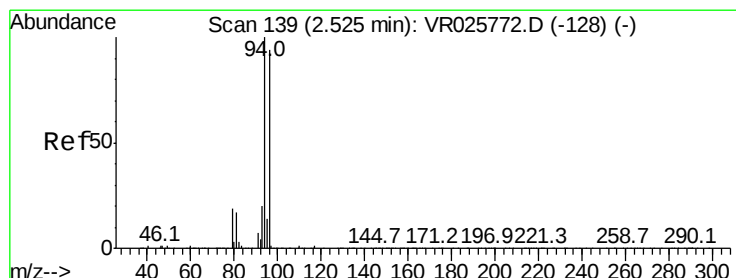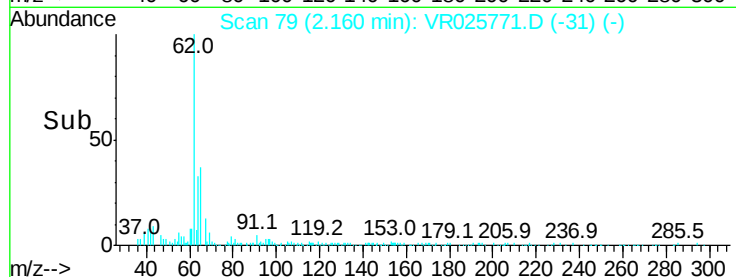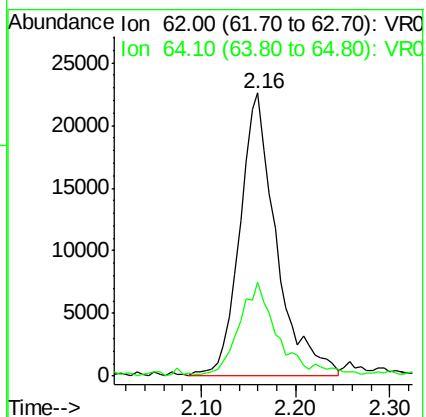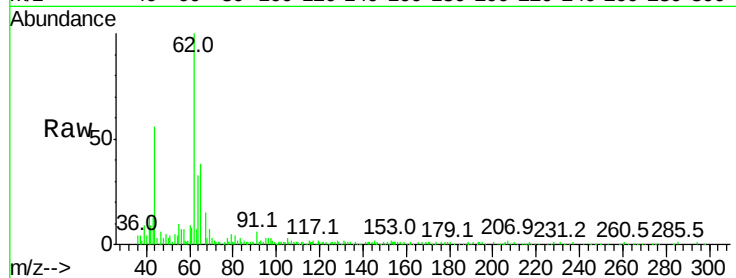

#6

Bromomethane

Concen: 1.265 ug/L

RT: 2.52 min Scan# 138

Delta R.T. -0.01 min

Lab File: VR025771.D

Acq: 20 Sep 2018 11:28

Tgt Ion: 94 Resp: 32499

Ion Ratio Lower Upper

94 100

96 88.1 66.1 122.7

