

#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 1.241 ug/L

RT: 3.67 min Scan# 328

Delta R.T. -0.00 min

Lab File: VR025771.D

Acq: 20 Sep 2018 11:28

Instrument :

MSVOA_R

ClientSampled :


Tgt Ion:101 Resp: 44260

Ion Ratio Lower Upper

101 100

85 49.8 37.6 56.4




151 75.3 60.9 91.3

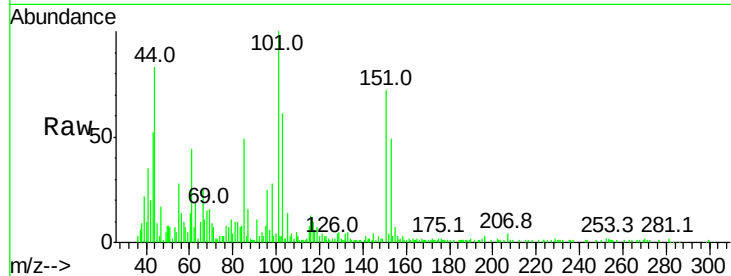

Abundance Ion 101.00 (100.70 to 101.70): V

Ion 85.00 (84.70 to 85.70): VR0

Ion 151.00 (150.70 to 151.70): V

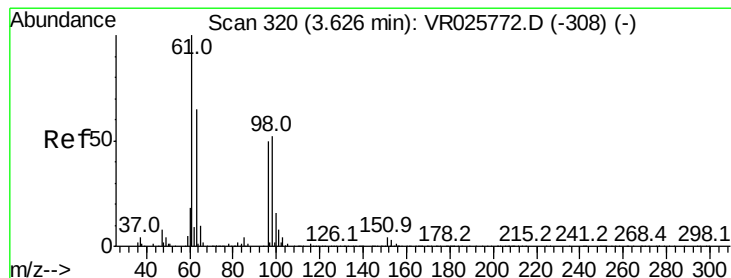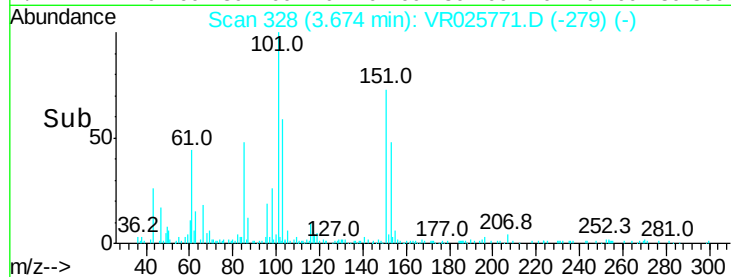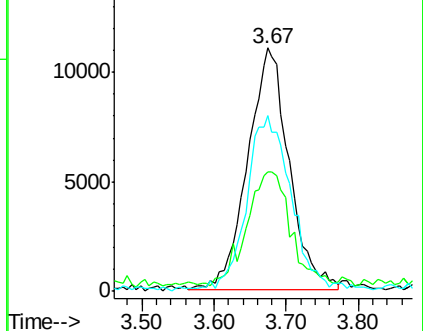

#12

1,1-Dichloroethene

Concen: 1.203 ug/L

RT: 3.63 min Scan# 320

Delta R.T. -0.00 min

Lab File: VR025771.D

Acq: 20 Sep 2018 11:28


Tgt Ion: 96 Resp: 45276

Ion Ratio Lower Upper

96 100

61 183.6 138.7 257.7

63 106.6 90.9 168.7

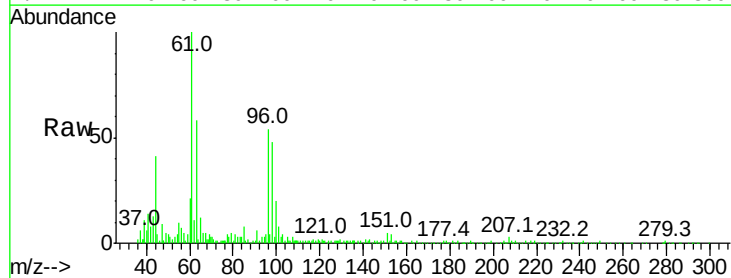

Abundance Ion 96.00 (95.70 to 96.70): VR0

Ion 61.05 (60.75 to 61.75): VR0

Ion 63.00 (62.70 to 63.70): VR0

