

#15

Methyl Acetate

Concen: 1.419 ug/L

RT: 4.19 min Scan# 413

Delta R.T. -0.00 min

Lab File: VR025771.D

Acq: 20 Sep 2018 11:28

Instrument :

MSVOA_R





ClientSampled :

Tgt Ion: 43 Resp: 8633

Ion Ratio Lower Upper

43 100

74 20.3 21.1 31.7#

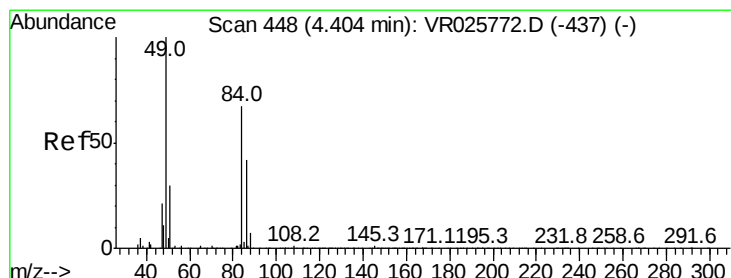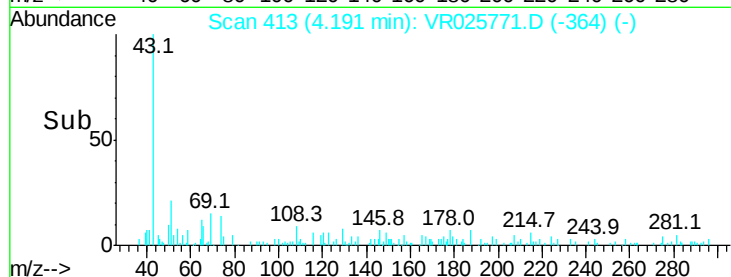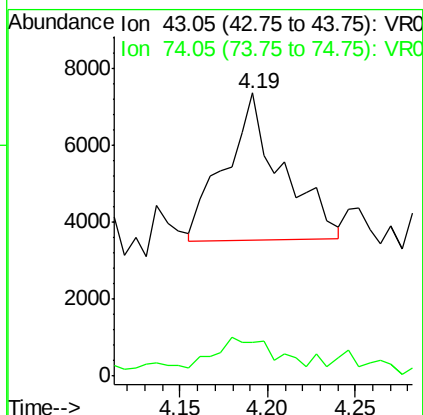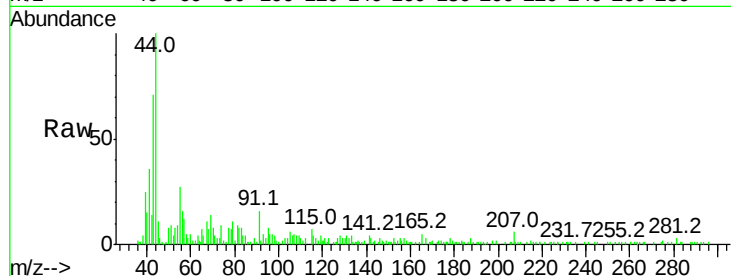

#16

Methylene chloride

Concen: 1.245 ug/L

RT: 4.40 min Scan# 447

Delta R.T. -0.01 min

Lab File: VR025771.D

Acq: 20 Sep 2018 11:28

Tgt Ion: 84 Resp: 41491

Ion Ratio Lower Upper

84 100

86 53.5 44.2 82.0

49 129.8 103.9 192.9

