
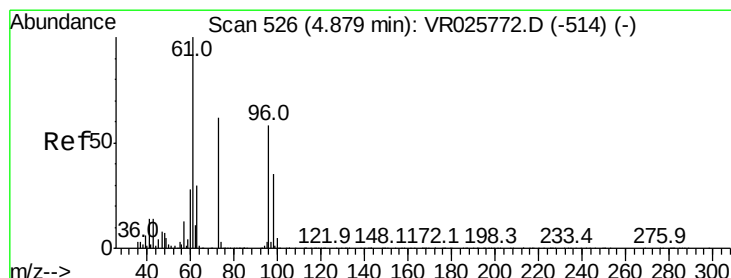
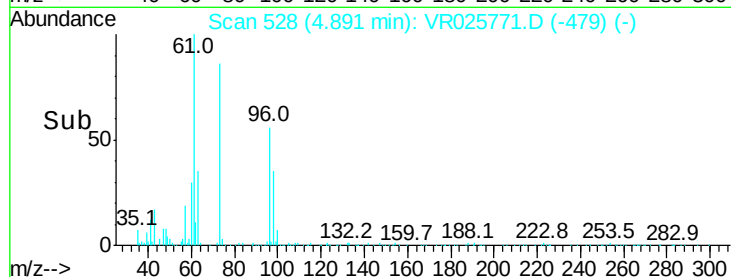
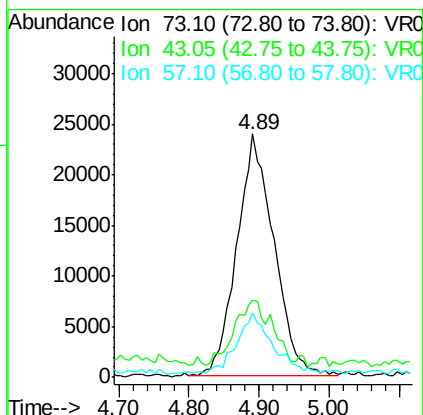


#17

Methyl tert-butyl Ether
 Concen: 1.904 ug/L
 RT: 4.89 min Scan# 528
 Delta R.T. -0.00 min
 Lab File: VR025771.D
 Acq: 20 Sep 2018 11:28

Instrument :
 MSVOA_R
 ClientSampleId :

Tgt Ion:	73	Resp:	88177
Ion	Ratio	Lower	Upper
73	100		
43	26.7	20.4	30.6
57	23.8	17.8	26.6

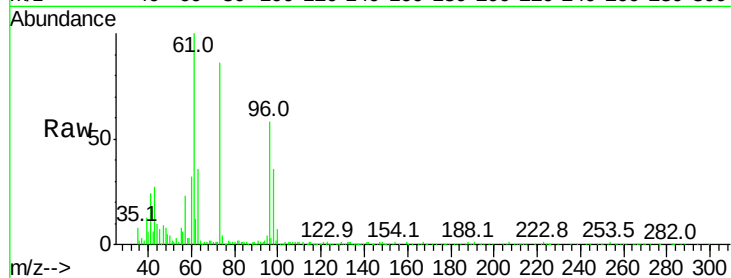

#18

trans-1,2-Dichloroethene
 Concen: 1.297 ug/L
 RT: 4.88 min Scan# 526
 Delta R.T. -0.00 min
 Lab File: VR025771.D
 Acq: 20 Sep 2018 11:28

Tgt Ion:	96	Resp:	59678
Ion	Ratio	Lower	Upper
96	100		
61	164.2	121.4	225.6
98	60.0	42.7	79.3

