

#19

1,1-Dichloroethane

Concen: 1.640 ug/L

RT: 5.69 min Scan# 660

Delta R.T. -0.00 min

Lab File: VR025771.D

Acq: 20 Sep 2018 11:28

Instrument :
MSVOA_R
ClientSampleId :





Tgt Ion: 63 Resp: 116324

Ion Ratio Lower Upper

63 100

65 30.6 22.7 42.1

83 11.5 9.3 17.3

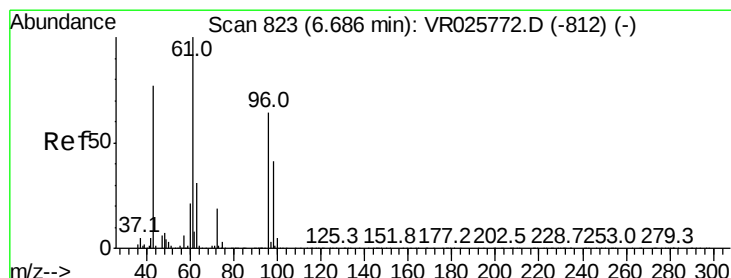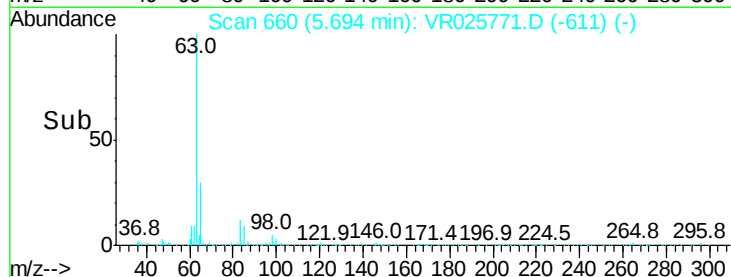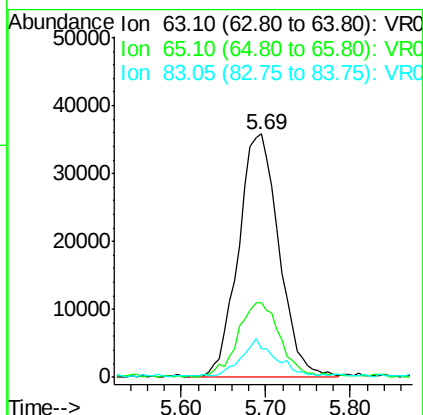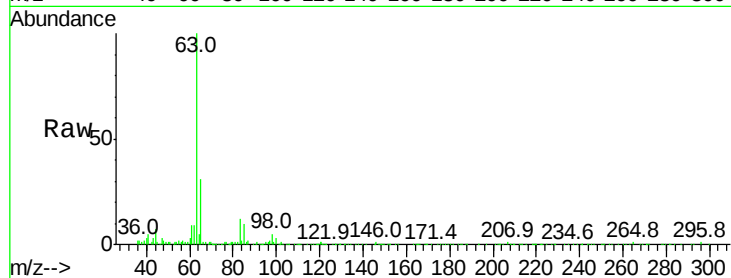

#21

2-Butanone

Concen: 16.673 ug/L

RT: 6.69 min Scan# 824

Delta R.T. 0.01 min

Lab File: VR025771.D

Acq: 20 Sep 2018 11:28

Tgt Ion: 43 Resp: 60050

Ion Ratio Lower Upper

43 100

72 23.4 12.4 37.0

