

#39

cis-1,3-Dichloropropene

Concen: 1.854 ug/L

RT: 9.72 min Scan# 1321

Delta R.T. -0.01 min





Lab File: VR025771.D

Acq: 20 Sep 2018 11:28

Instrument :
MSVOA_R
ClientSampleId :

Tgt Ion: 75 Resp: 71302

Ion	Ratio	Lower	Upper
75	100		
77	28.1	21.2	39.4

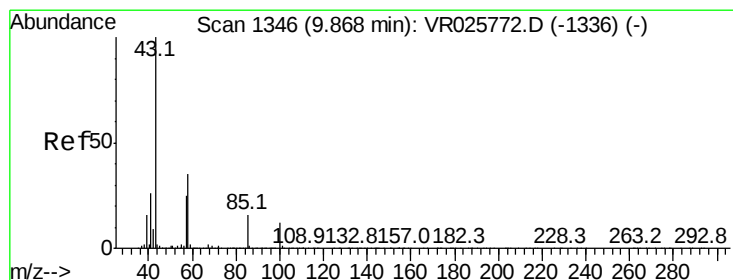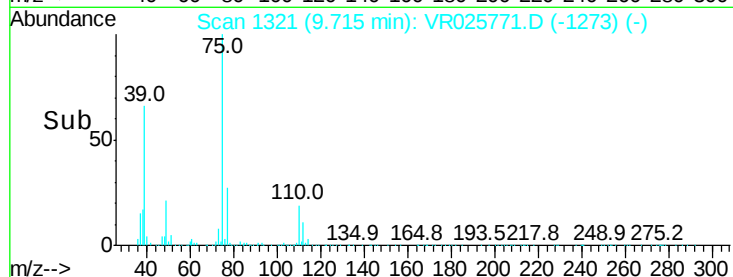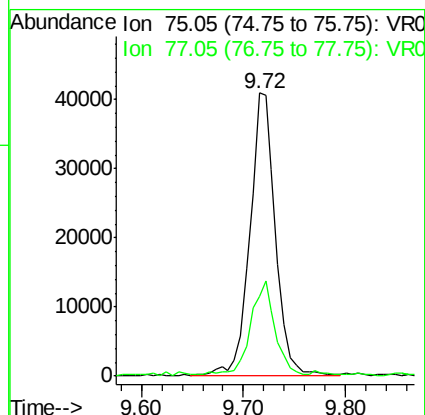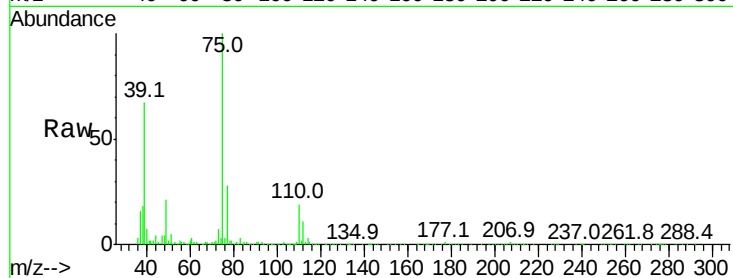

#40

4-Methyl-2-pentanone

Concen: 19.286 ug/L

RT: 9.87 min Scan# 1346

Delta R.T. -0.00 min

Lab File: VR025771.D

Acq: 20 Sep 2018 11:28

Tgt Ion: 43 Resp: 179262

Ion	Ratio	Lower	Upper
43	100		
58	35.7	28.3	42.5
100	11.6	9.3	13.9

