

#42

Toluene

Concen: 1.381 ug/L

RT: 10.03 min Scan# 1373

Delta R.T. -0.00 min

Lab File: VR025771.D

Acq: 20 Sep 2018 11:28

Instrument :

MSVOA_R





ClientSampleId :

Tgt Ion: 91 Resp: 235823

Ion Ratio Lower Upper

91 100

92 58.8 41.1 76.3

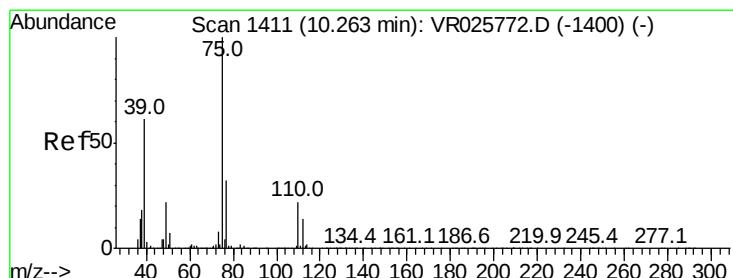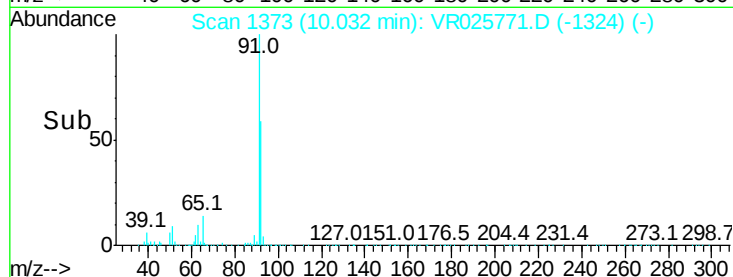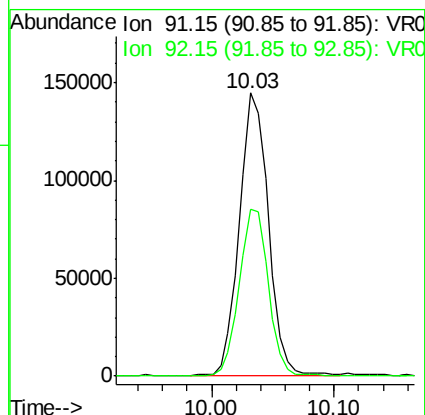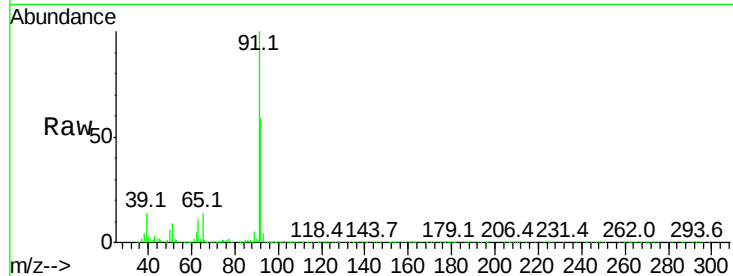

#44

trans-1,3-Dichloropropene

Concen: 1.904 ug/L

RT: 10.26 min Scan# 1411

Delta R.T. -0.00 min

Lab File: VR025771.D

Acq: 20 Sep 2018 11:28

Tgt Ion: 75 Resp: 51498

Ion Ratio Lower Upper

75 100

77 30.9 22.6 42.0

