
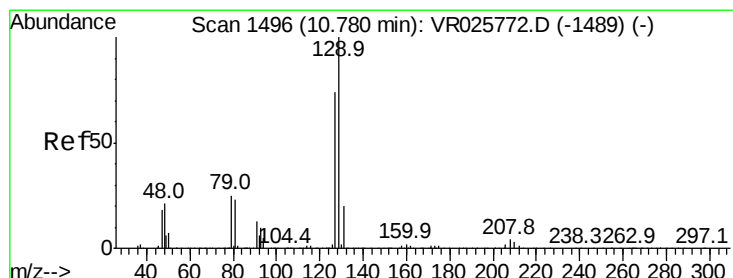
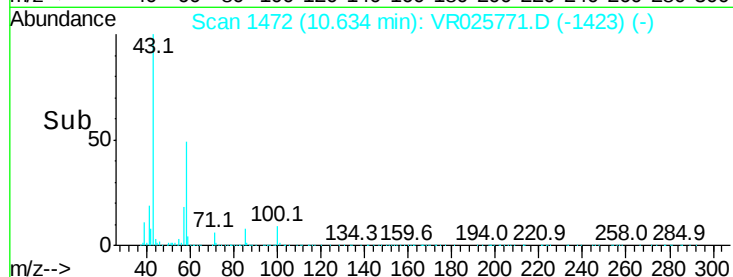
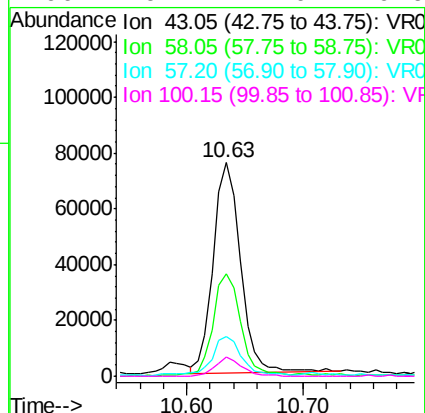


#48
2-Hexanone
Concen: 18.567 ug/L
RT: 10.63 min Scan# 1472
Delta R.T. -0.00 min
Lab File: VR025771.D
Acq: 20 Sep 2018 11:28

Instrument :
MSVOA_R
ClientSampleId :

Tgt Ion:	43	Resp:	121032
Ion	Ratio	Lower	Upper
43	100		
58	50.0	39.9	59.9
57	20.8	14.3	21.5
100	9.2	7.0	10.6

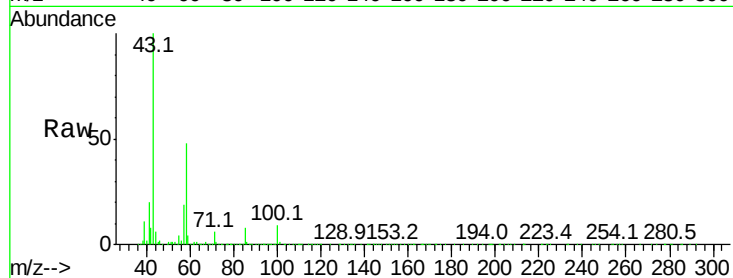

#49
Dibromochloromethane
Concen: 1.414 ug/L
RT: 10.79 min Scan# 1497
Delta R.T. 0.01 min
Lab File: VR025771.D
Acq: 20 Sep 2018 11:28

Tgt Ion:	129	Resp:	26537
Ion	Ratio	Lower	Upper
129	100		
127	77.6	51.9	96.5

