

#52

Ethylbenzene

Concen: 1.558 ug/L

RT: 11.39 min Scan# 1597

Delta R.T. -0.00 min

Lab File: VR025771.D

Acq: 20 Sep 2018 11:28

Instrument :

MSVOA\_R


ClientSampleId :

Tgt Ion: 91 Resp: 286525

Ion Ratio Lower Upper




91 100

106 29.4 21.4 39.8

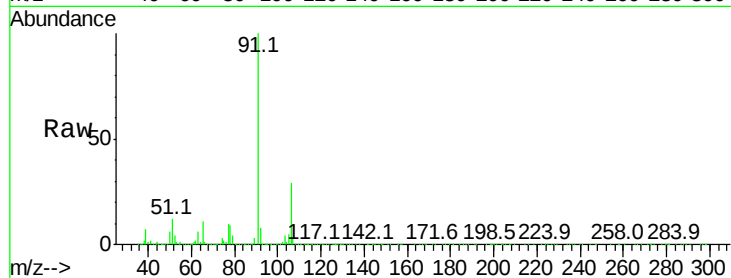

Abundance Ion 91.15 (90.85 to 91.85): VR0

Ion 106.15 (105.85 to 106.85): V

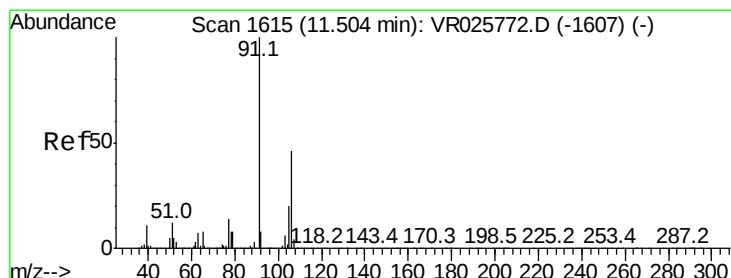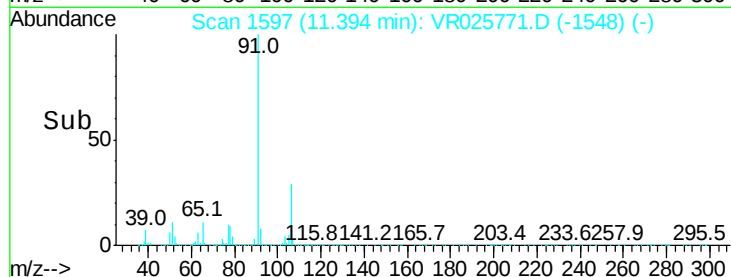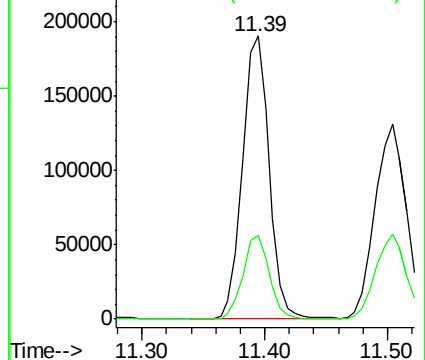

#53

m,p-Xylene

Concen: 1.331 ug/L

RT: 11.50 min Scan# 1615

Delta R.T. -0.00 min

Lab File: VR025771.D


Acq: 20 Sep 2018 11:28

Tgt Ion: 106 Resp: 98540

Ion Ratio Lower Upper

106 100

91 228.3 154.3 286.5

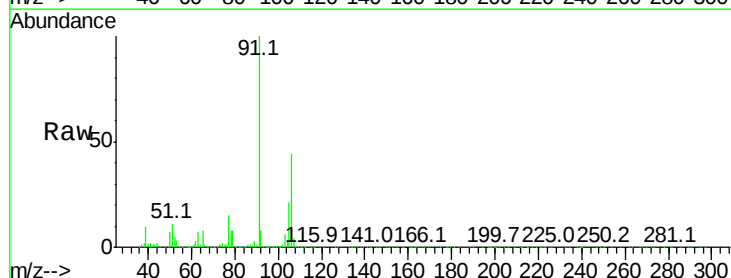

Abundance Ion 106.15 (105.85 to 106.85): V

Ion 91.15 (90.85 to 91.85): VR0

