

#56

Isopropylbenzene

Concen: 1.639 ug/L

RT: 12.13 min Scan# 1718

Delta R.T. -0.00 min

Lab File: VR025771.D


Acq: 20 Sep 2018 11:28

Instrument :

MSVOA_R

ClientSampled :




Tgt Ion:	105	Resp:	266345
Ion Ratio	Lower	Upper	
105	100		
120	25.7	20.1	30.1
77	18.9	15.3	22.9

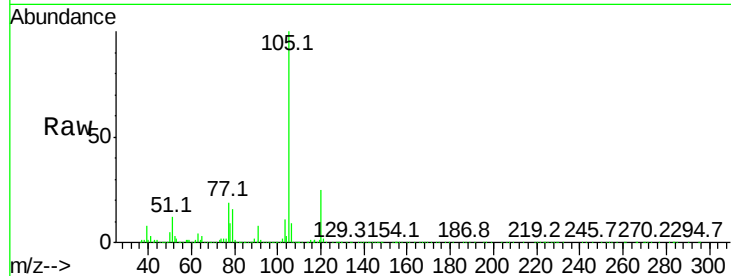

Abundance Ion 105.05 (104.75 to 105.75): V

Ion 120.10 (119.80 to 120.80): V

Ion 77.10 (76.80 to 77.80): VR0

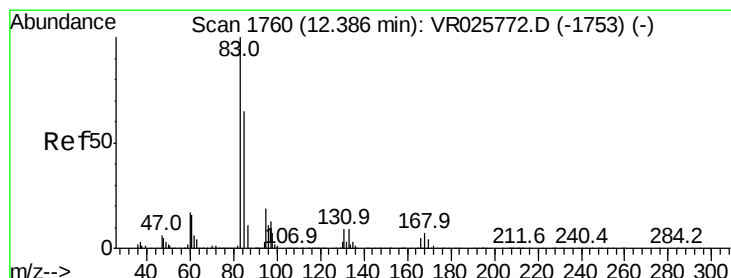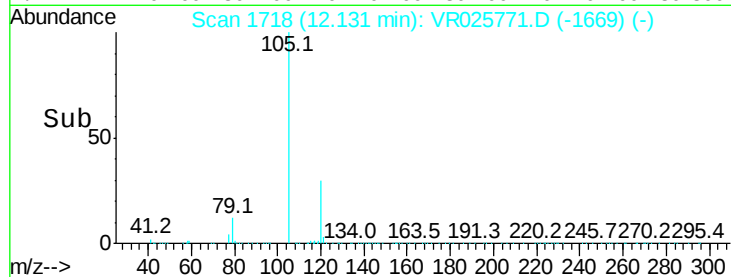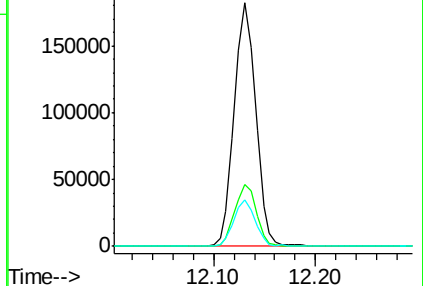

#58

1,1,2,2-Tetrachloroethane

Concen: 1.386 ug/L


RT: 12.39 min Scan# 1760

Delta R.T. -0.00 min

Lab File: VR025771.D

Acq: 20 Sep 2018 11:28

Tgt Ion:	83	Resp:	23781
Ion Ratio	Lower	Upper	
83	100		
85	60.2	45.4	84.4
131	12.5	7.5	11.3#

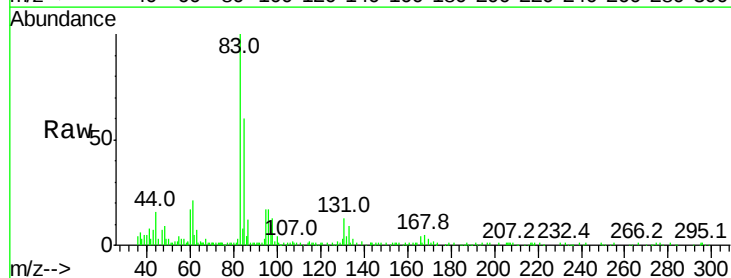

Abundance Ion 82.95 (82.65 to 83.65): VR0

Ion 85.00 (84.70 to 85.70): VR0

Ion 130.95 (130.65 to 131.65): V

