

#59

1,2,3-Trichloropropane

Concen: 1.670 ug/L

RT: 12.43 min Scan# 1768

Delta R.T. -0.00 min

Lab File: VR025771.D

Acq: 20 Sep 2018 11:28

Instrument :

MSVOA_R





ClientSampled :

Tgt Ion: 75 Resp: 19264

Ion Ratio Lower Upper

75 100

77 31.0 25.6 38.4

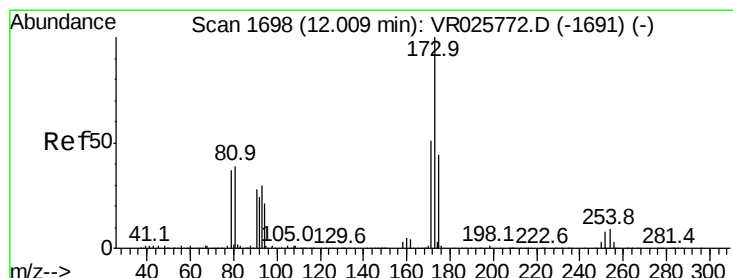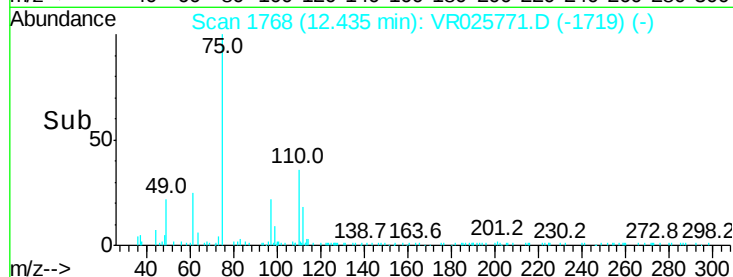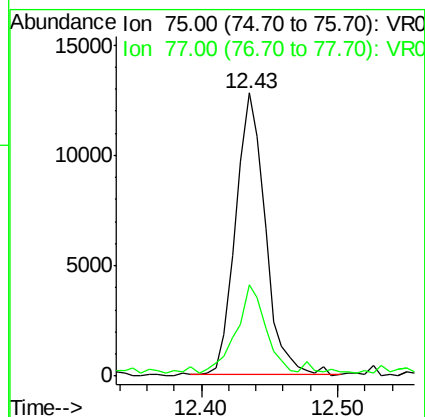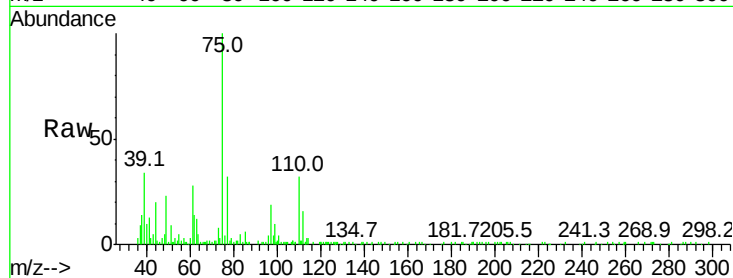

#61

Bromoform

Concen: 1.412 ug/L

RT: 12.01 min Scan# 1698

Delta R.T. -0.00 min

Lab File: VR025771.D

Acq: 20 Sep 2018 11:28

Tgt Ion: 173 Resp: 10596

Ion Ratio Lower Upper

173 100

175 56.7 39.9 59.9

254 9.6 6.6 9.8

