

#62

1,3-Dichlorobenzene

Concen: 1.484 ug/L

RT: 13.16 min Scan# 1887

Delta R.T. -0.01 min

Lab File: VR025771.D


Acq: 20 Sep 2018 11:28

Instrument :

MSVOA_R

ClientSampled :




Tgt Ion:	146	Resp:	81354
Ion	Ratio	Lower	Upper
146	100		
111	48.7	32.1	59.5
148	56.8	44.3	82.3

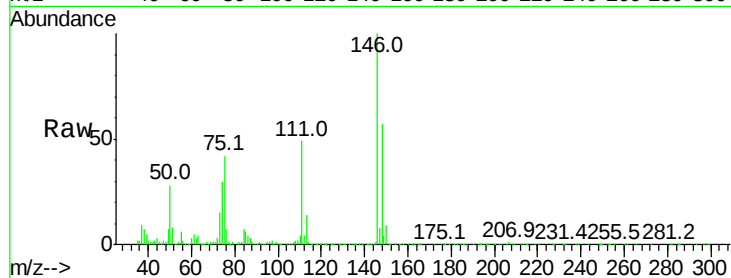

Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

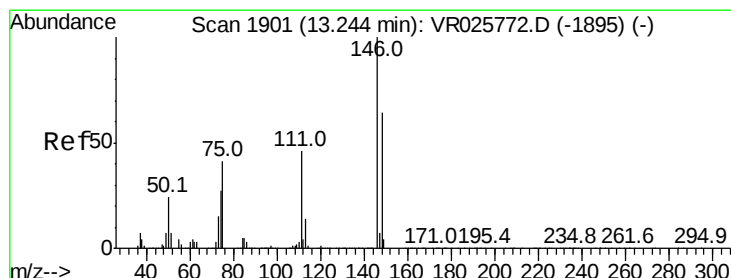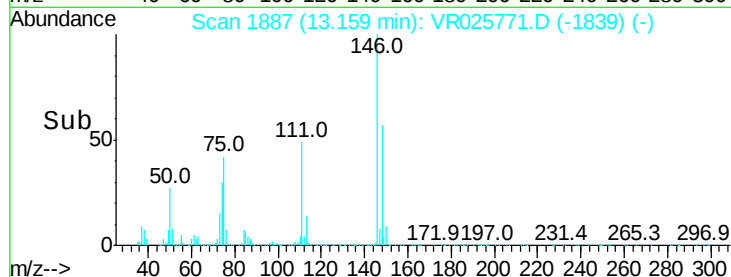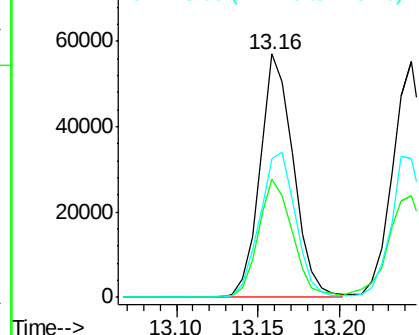

#63

1,4-Dichlorobenzene

Concen: 1.268 ug/L


RT: 13.24 min Scan# 1901

Delta R.T. -0.00 min

Lab File: VR025771.D

Acq: 20 Sep 2018 11:28

Tgt Ion:	146	Resp:	79008
Ion	Ratio	Lower	Upper
146	100		
111	43.3	32.3	60.1
148	59.1	44.6	82.8

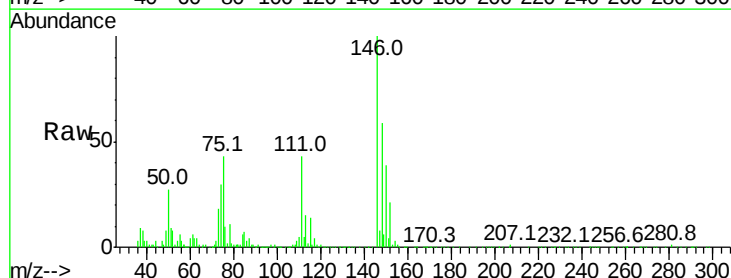

Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

