

#69

Naphthalene

Concen: 2.084 ug/L

RT: 15.00 min Scan# 2190

Delta R.T. -0.00 min

Lab File: VR025771.D





Acq: 20 Sep 2018 11:28

Instrument :

MSVOA_R

ClientSampleId :

Tgt Ion:	128	Resp:	46587
Ion	Ratio	Lower	Upper
128	100		
127	12.4	10.3	15.5
129	11.2	9.1	13.7

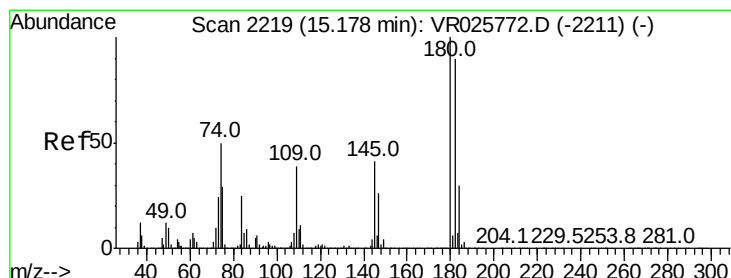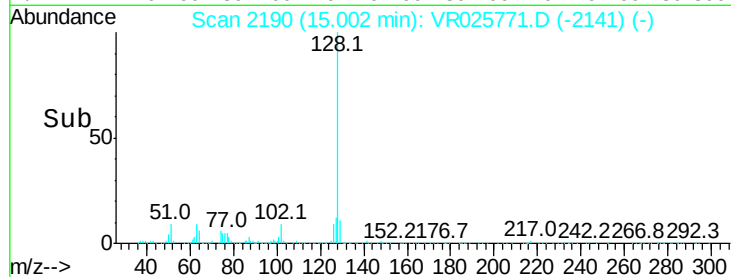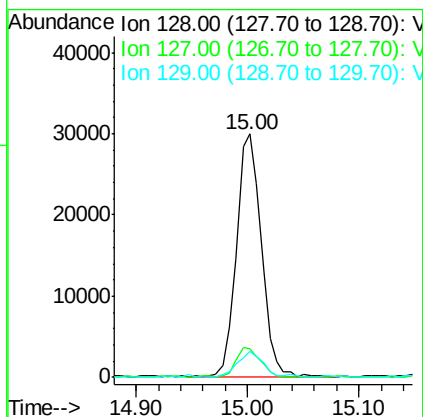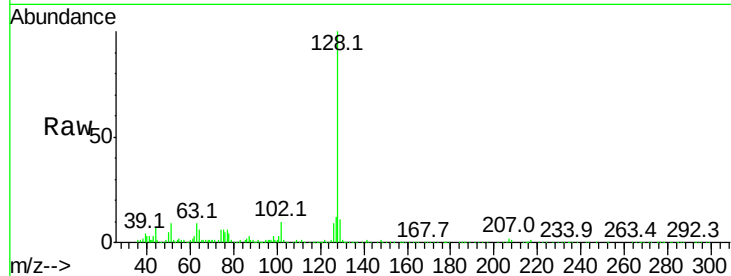

#70

1,2,3-Trichlorobenzene

Concen: 1.424 ug/L

RT: 15.18 min Scan# 2219

Delta R.T. -0.00 min

Lab File: VR025771.D

Acq: 20 Sep 2018 11:28

Tgt Ion:	180	Resp:	22533
Ion	Ratio	Lower	Upper
180	100		
182	91.8	75.7	113.5
145	39.0	31.8	47.8

