

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR100118\
 Data File : VR025917.D
 Acq On : 1 Oct 2018 17:54
 Operator : SY/MD
 Sample : J5160-01
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 GACA6

Quant Time: Oct 02 01:48:05 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 02 01:45:34 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	463667	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	388233	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	131451	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.15	65	153231	4.19	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.80%
7) Chloroethane-d5	2.63	69	139200	4.66	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.20%
11) 1,1-Dichloroethene-d2	3.63	63	275238	3.21	ug/L	0.01
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.20%
20) 2-Butanone-d5	6.59	46	257621	63.20	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	126.40%
24) Chloroform-d	7.20	84	302056	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.00%
26) 1,2-Dichloroethane-d4	7.90	65	137783	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.60%
32) Benzene-d6	7.85	84	577522	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.40%
36) 1,2-Dichloropropane-d6	8.90	67	170973	4.91	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.20%
41) Toluene-d8	9.97	98	502895	4.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.80%
43) trans-1,3-Dichloropropene-	10.24	79	36526	4.62	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.40%
46) 2-Hexanone-d5	10.59	63	183525	60.89	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	121.78%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	70695	5.00	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.00%
64) 1,2-Dichlorobenzene-d4	13.51	152	104987	4.99	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.80%

Target Compounds


					Ovalue
15) Methyl Acetate	4.19	43	1080	0.132 ug/L #	76
25) Chloroform	7.22	83	13682	0.245 ug/L	89
31) Carbon tetrachloride	7.63	117	243233	6.433 ug/L	99
34) Trichloroethene	8.46	95	15329	0.447 ug/L #	14
35) Methylcyclohexane	8.90	83	39797	0.771 ug/L #	16
37) 1,2-Dichloropropane	8.90	63	20834	0.746 ug/L #	95
44) trans-1,3-Dichloropropene	10.23	75	2413	0.118 ug/L	95
48) 2-Hexanone	10.59	43	27388	4.259 ug/L #	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA R\DATA\VR100118\
Data File : VR025917.D
Acq On : 1 Oct 2018 17:54
Operator : SY/MD
Sample : J5160-01
Misc : 25mL/MSVOA R/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
GACA6

Quant Time: Oct 02 01:48:05 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 02 01:45:34 2018
Response via : Initial Calibration




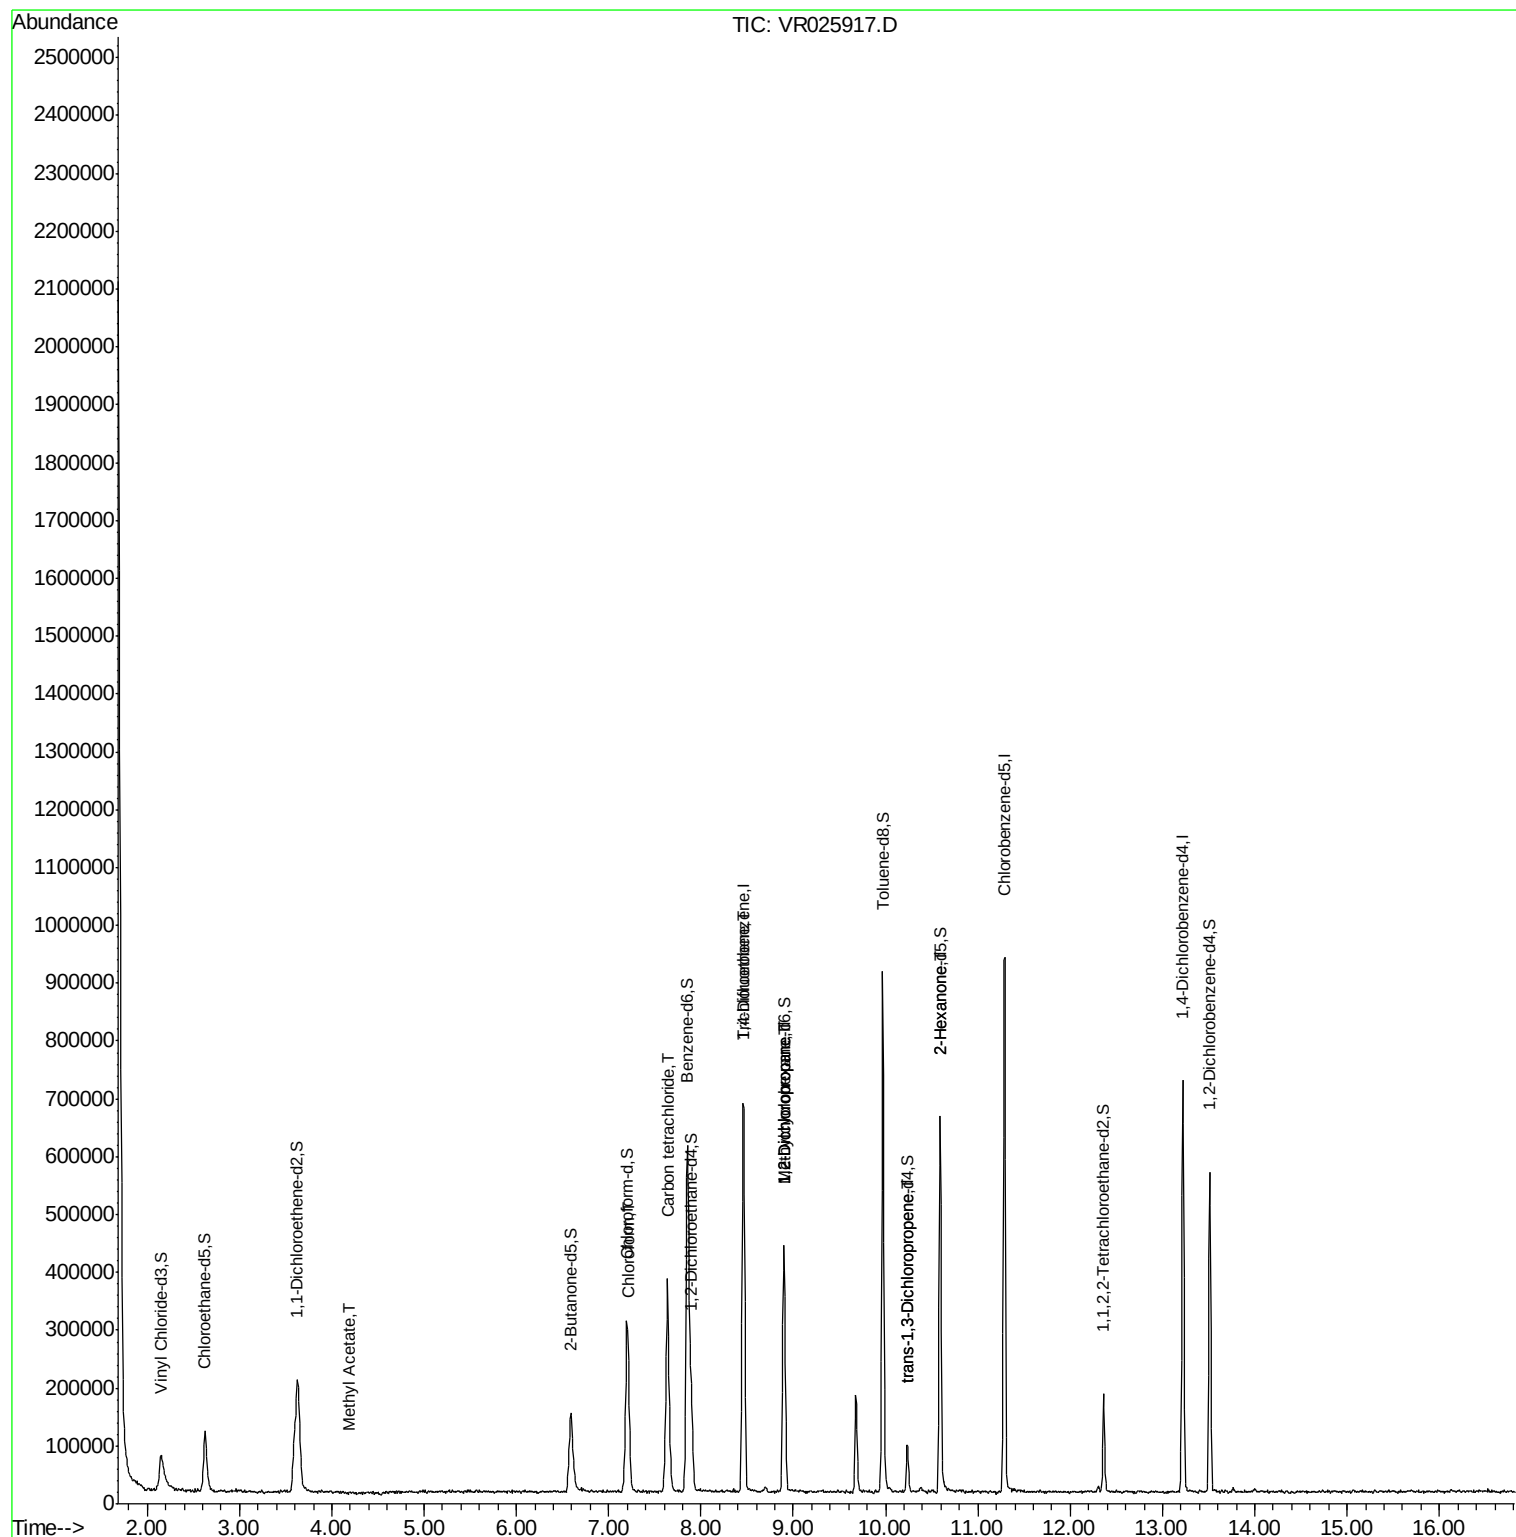


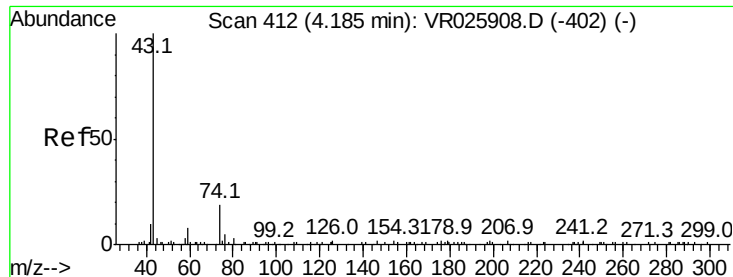

#15
Methyl Acetate
Concen: 0.132 ug/L
RT: 4.19 min Scan# 412
Delta R.T. 0.00 min
Lab File: VR025917.D
Acq: 1 Oct 2018 17:54




Instrument :
MSVOA_R
ClientSampled :
GACA6


Tot Ion: 43 Resp: 1080
Ion Ratio Lower Upper
43 100
74 12.0 19.0 28.4#

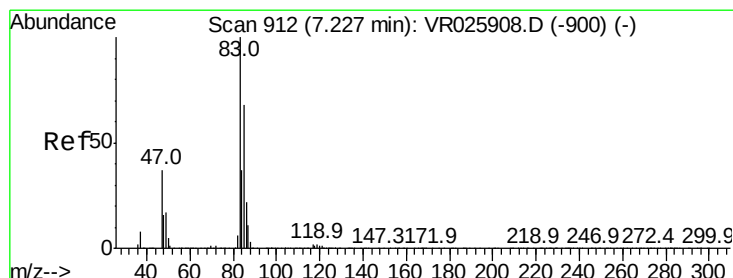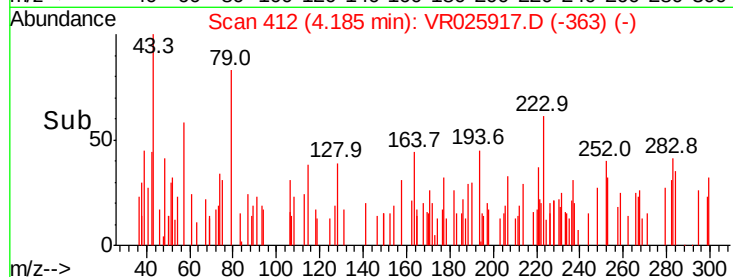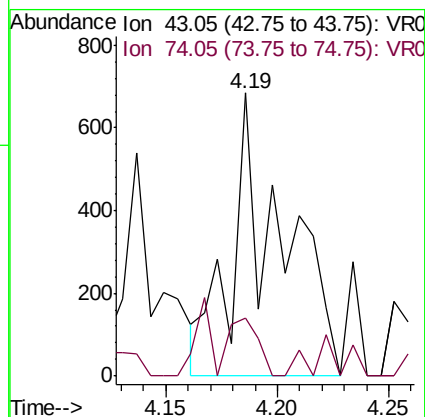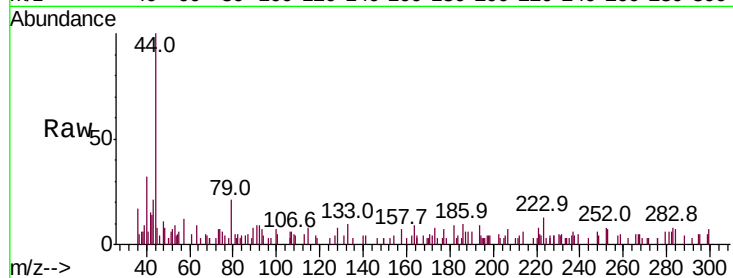

#25
Chloroform
Concen: 0.245 ug/L
RT: 7.22 min Scan# 911
Delta R.T. -0.01 min
Lab File: VR025917.D
Acq: 1 Oct 2018 17:54

Tgt Ion: 83 Resp: 13682
Ion Ratio Lower Upper
83 100
85 70.8 43.8 81.4

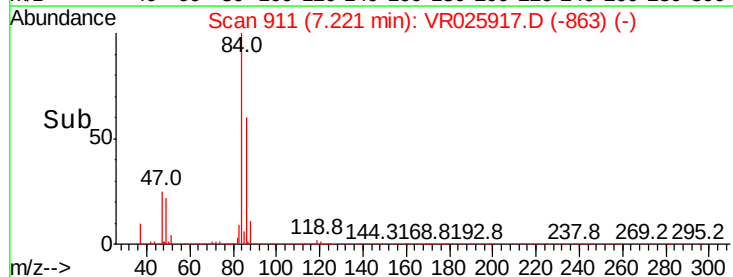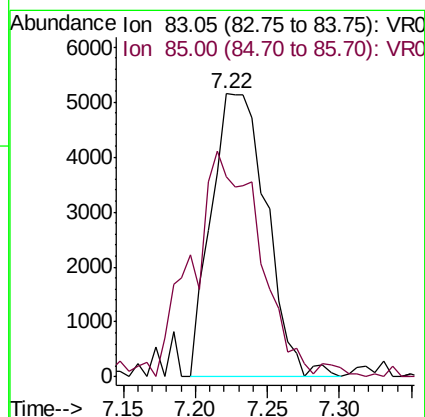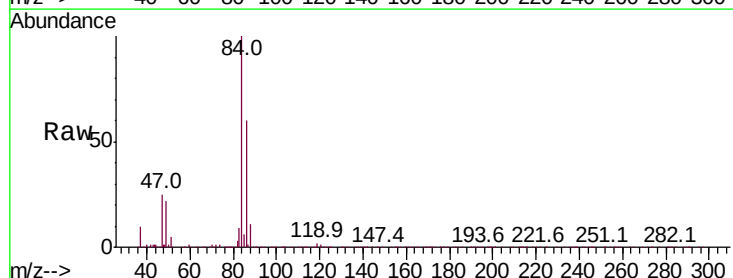

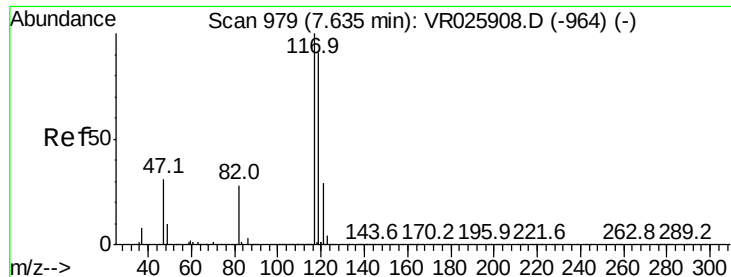

#31

Carbon tetrachloride

Concen: 6.433 ug/L

RT: 7.63 min Scan# 979

Delta R.T. 0.00 min

Lab File: VR025917.D

Acq: 1 Oct 2018 17:54

Instrument :

MSVOA_R

ClientSampled :


GACA6

Tot Ion:117 Resp: 243233

Ion Ratio Lower Upper




117 100

119 95.1 75.6 113.4

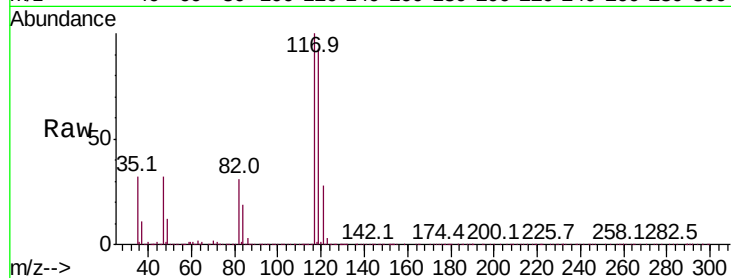

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 118.90 (118.60 to 119.60): V

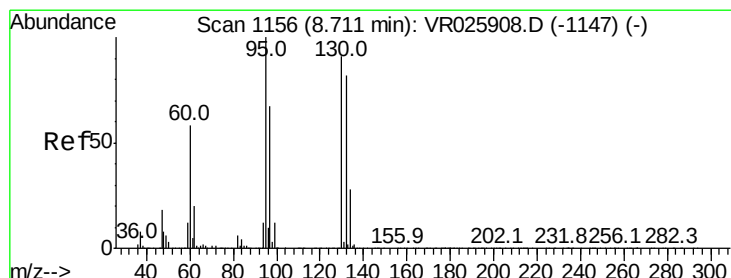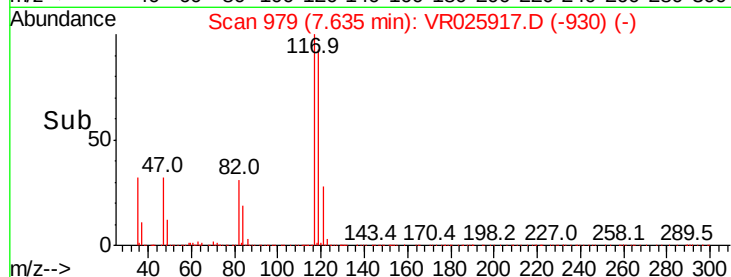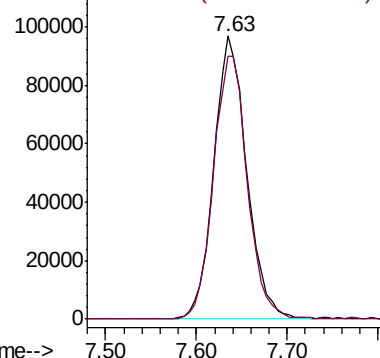

#34

Trichloroethene

Concen: 0.447 ug/L

RT: 8.46 min Scan# 1115

Delta R.T. -0.25 min

Lab File: VR025917.D

Acq: 1 Oct 2018 17:54

Tgt Ion: 95 Resp: 15329


Ion Ratio Lower Upper

95 100

97 1.7 43.9 81.5#

132 0.7 53.3 98.9#

130 0.0 53.8 99.8#


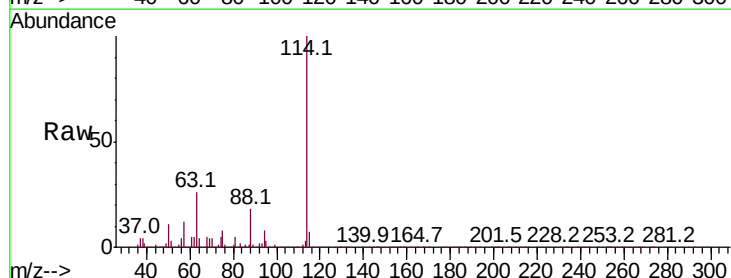



Abundance Ion 95.00 (94.70 to 95.70): VR0

Ion 96.95 (96.65 to 97.65): VR0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V



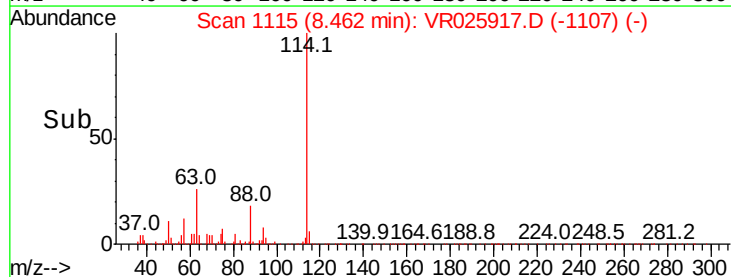
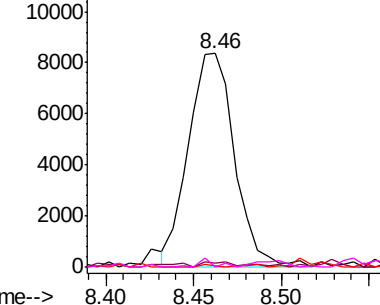


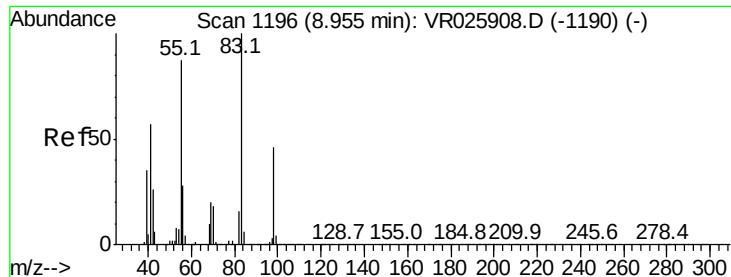

#35
Methylcyclohexane
Concen: 0.771 ug/L
RT: 8.90 min Scan# 1187
Delta R.T. -0.05 min
Lab File: VR025917.D
Acq: 1 Oct 2018 17:54




Instrument :
MSVOA_R
ClientSampled :
GACA6


Tot Ion: 83 Resp: 39797
Ion Ratio Lower Upper
83 100
55 1.2 71.8 107.6#
98 1.8 34.2 51.4#

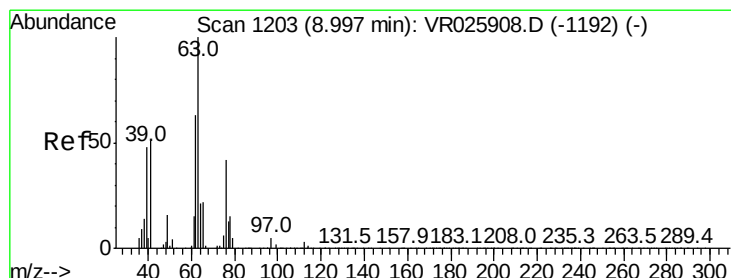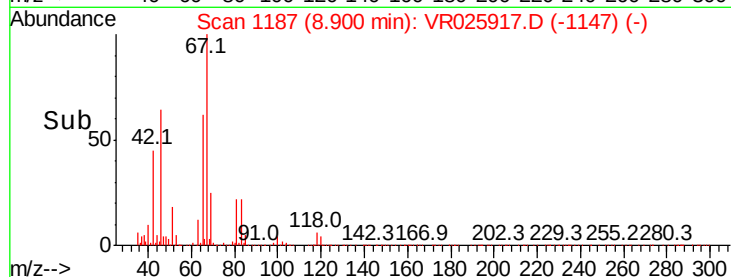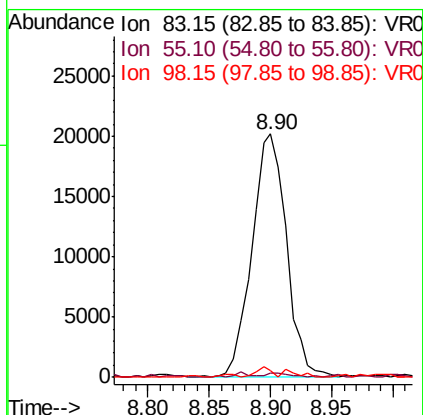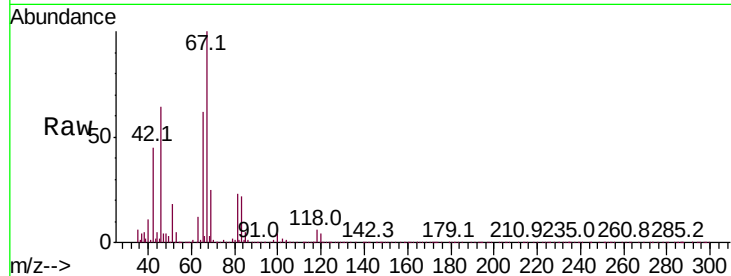

#37
1,2-Dichloropropane
Concen: 0.746 ug/L
RT: 8.90 min Scan# 1187
Delta R.T. -0.10 min
Lab File: VR025917.D
Acq: 1 Oct 2018 17:54

Tgt Ion: 63 Resp: 20834
Ion Ratio Lower Upper
63 100
112 1.4 2.5 3.7#

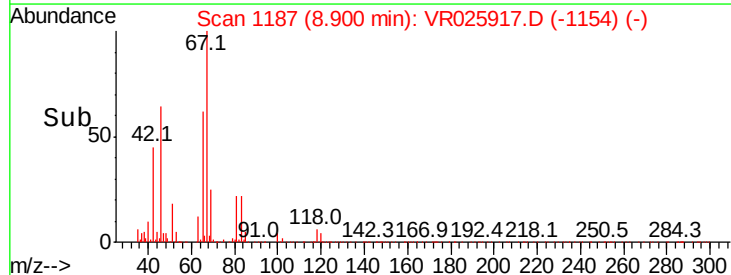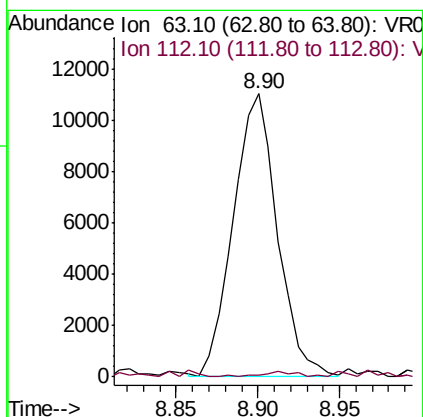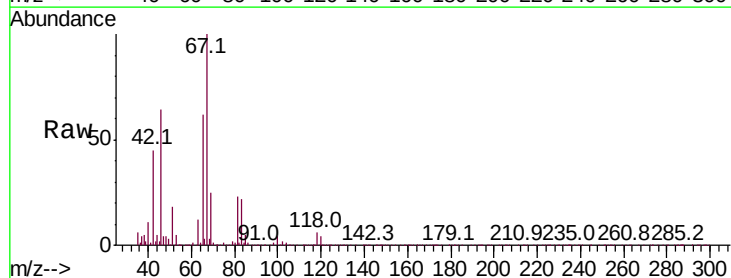

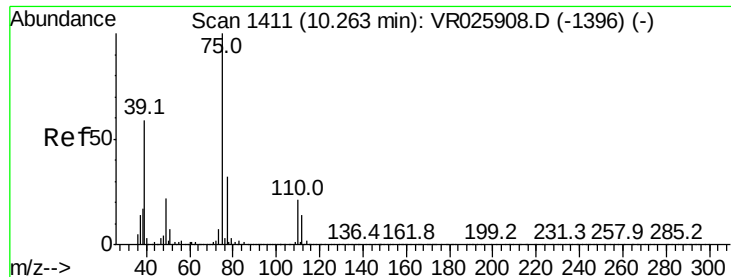

#44

trans-1,3-Dichloropropene

Concen: 0.118 ug/L

RT: 10.23 min Scan# 1406

Delta R.T. -0.03 min

Lab File: VR025917.D

Acq: 1 Oct 2018 17:54

Instrument :

MSVOA_R

ClientSampleId :





GACA6

Tot Ion: 75 Resp: 2413

Ion Ratio Lower Upper

75 100

77 30.0 23.0 42.8

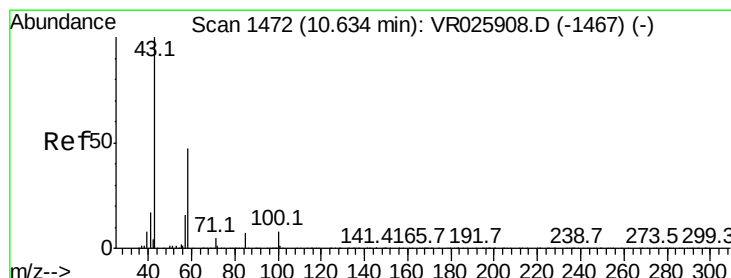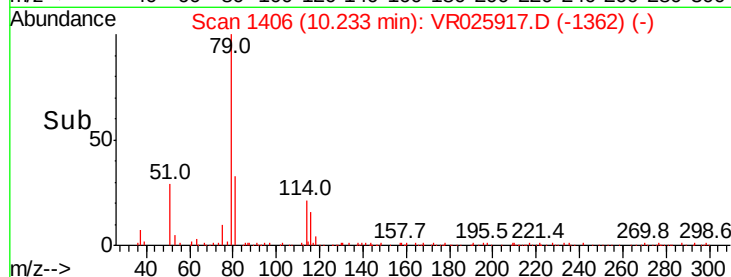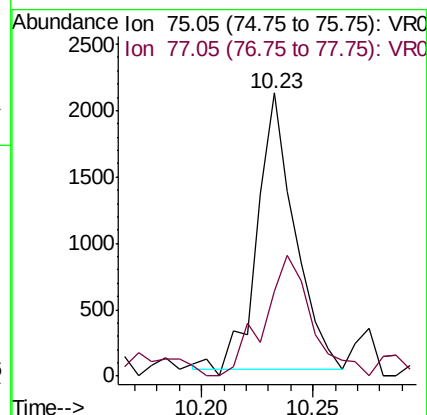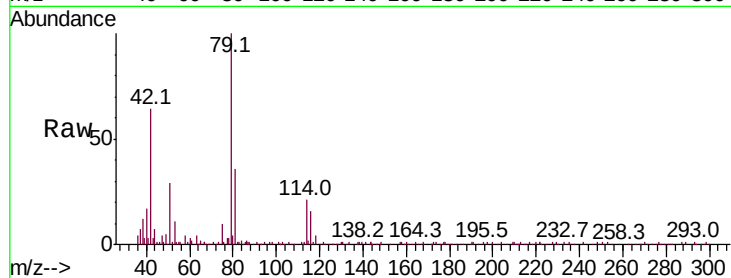

#48

2-Hexanone

Concen: 4.259 ug/L

RT: 10.59 min Scan# 1465

Delta R.T. -0.04 min

Lab File: VR025917.D

Acq: 1 Oct 2018 17:54

Tgt Ion: 43 Resp: 27388

Ion Ratio Lower Upper

43 100

58 24.1 39.5 59.3#

57 24.9 14.6 21.8#

100 1.5 6.7 10.1#

