

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR100118\
 Data File : VR025914.D
 Acq On : 1 Oct 2018 16:15
 Operator : SY/MD
 Sample : J5073-02
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 ET0T1

Quant Time: Oct 02 02:05:51 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 02 01:45:34 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	482614	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	396009	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	135515	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.15	65	191833	5.04	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.80%
7) Chloroethane-d5	2.63	69	162448	5.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.40%
11) 1,1-Dichloroethene-d2	3.63	63	316340	3.54	ug/L	0.01
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.80%
20) 2-Butanone-d5	6.59	46	254423	59.97	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.94%
24) Chloroform-d	7.20	84	323318	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.60%
26) 1,2-Dichloroethane-d4	7.90	65	146728	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.00%
32) Benzene-d6	7.85	84	638052	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
36) 1,2-Dichloropropane-d6	8.90	67	181838	5.12	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.40%
41) Toluene-d8	9.97	98	566394	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.40%
43) trans-1,3-Dichloropropene-	10.24	79	39259	4.87	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.40%
46) 2-Hexanone-d5	10.59	63	185801	60.43	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	120.86%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	74499	5.17	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.40%
64) 1,2-Dichlorobenzene-d4	13.51	152	114994	5.30	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.00%


Target Compounds					Ovalue
13) Acetone	3.70	43	72338	23.523 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR100118\
Data File : VR025914.D
Acq On : 1 Oct 2018 16:15
Operator : SY/MD
Sample : J5073-02
Misc : 25mL/MSVOA R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
ET0T1

Quant Time: Oct 02 02:05:51 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 02 01:45:34 2018
Response via : Initial Calibration

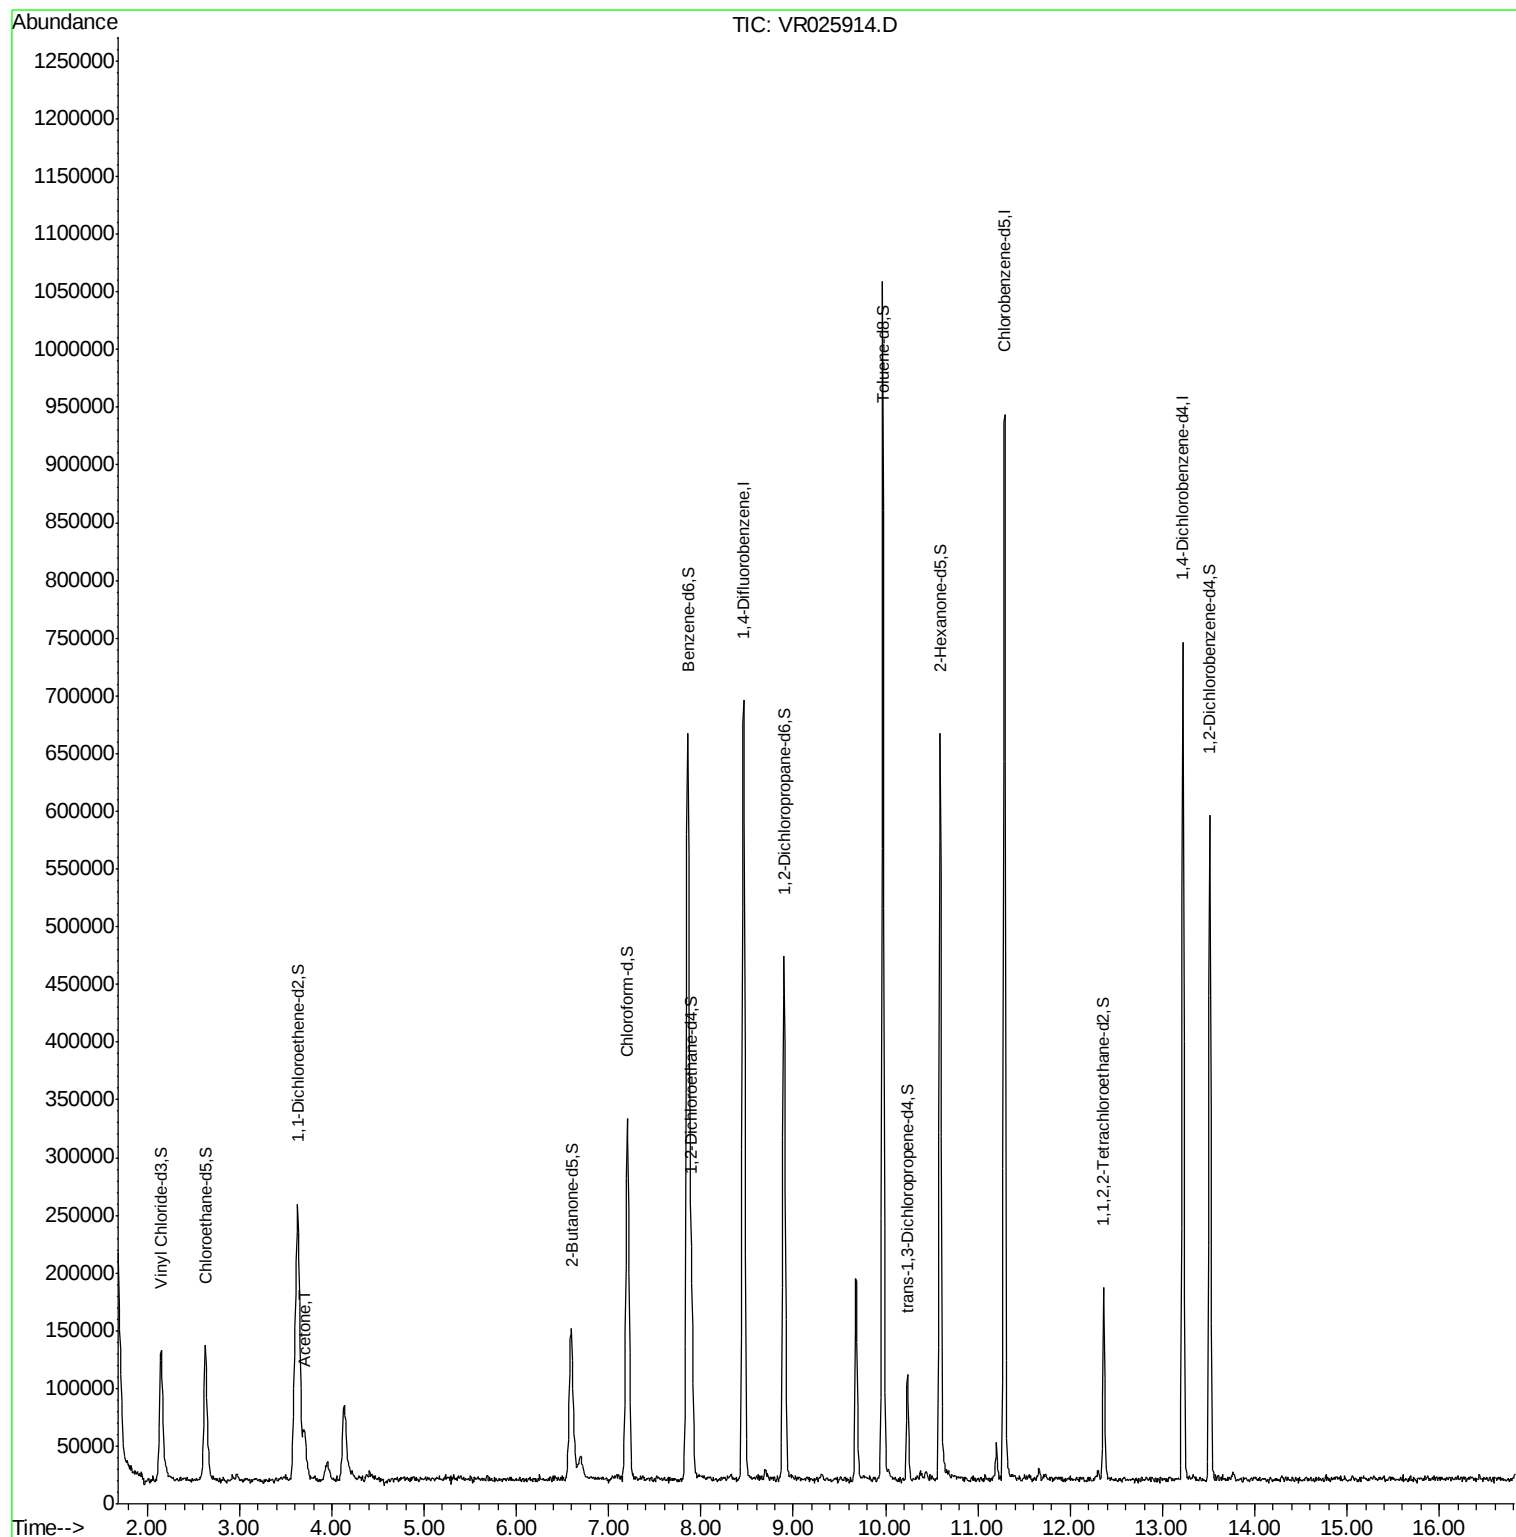

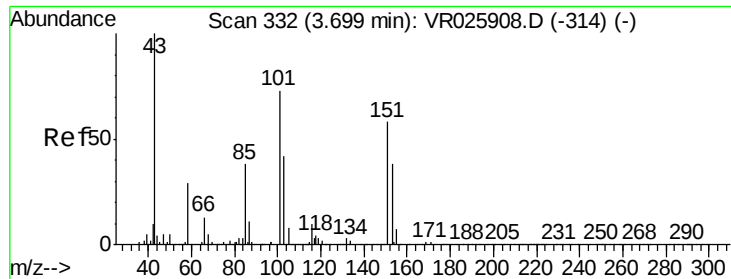

#13

Acetone

Concen: 23.523 ug/L

RT: 3.70 min Scan# 332

Delta R.T. 0.00 min

Lab File: VR025914.D

Acq: 1 Oct 2018 16:15

Instrument :
MSVOA_R
ClientSampleId :
ET0T1

Tot Ion: 43 Resp: 72338

Ion Ratio Lower Upper

43 100

58 29.0 0.0 51.4

