


Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR100218\
 Data File : VR025920.D
 Acq On : 2 Oct 2018 9:40
 Operator : SY/MD
 Sample : BFB80
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Oct 04 08:45:53 2018

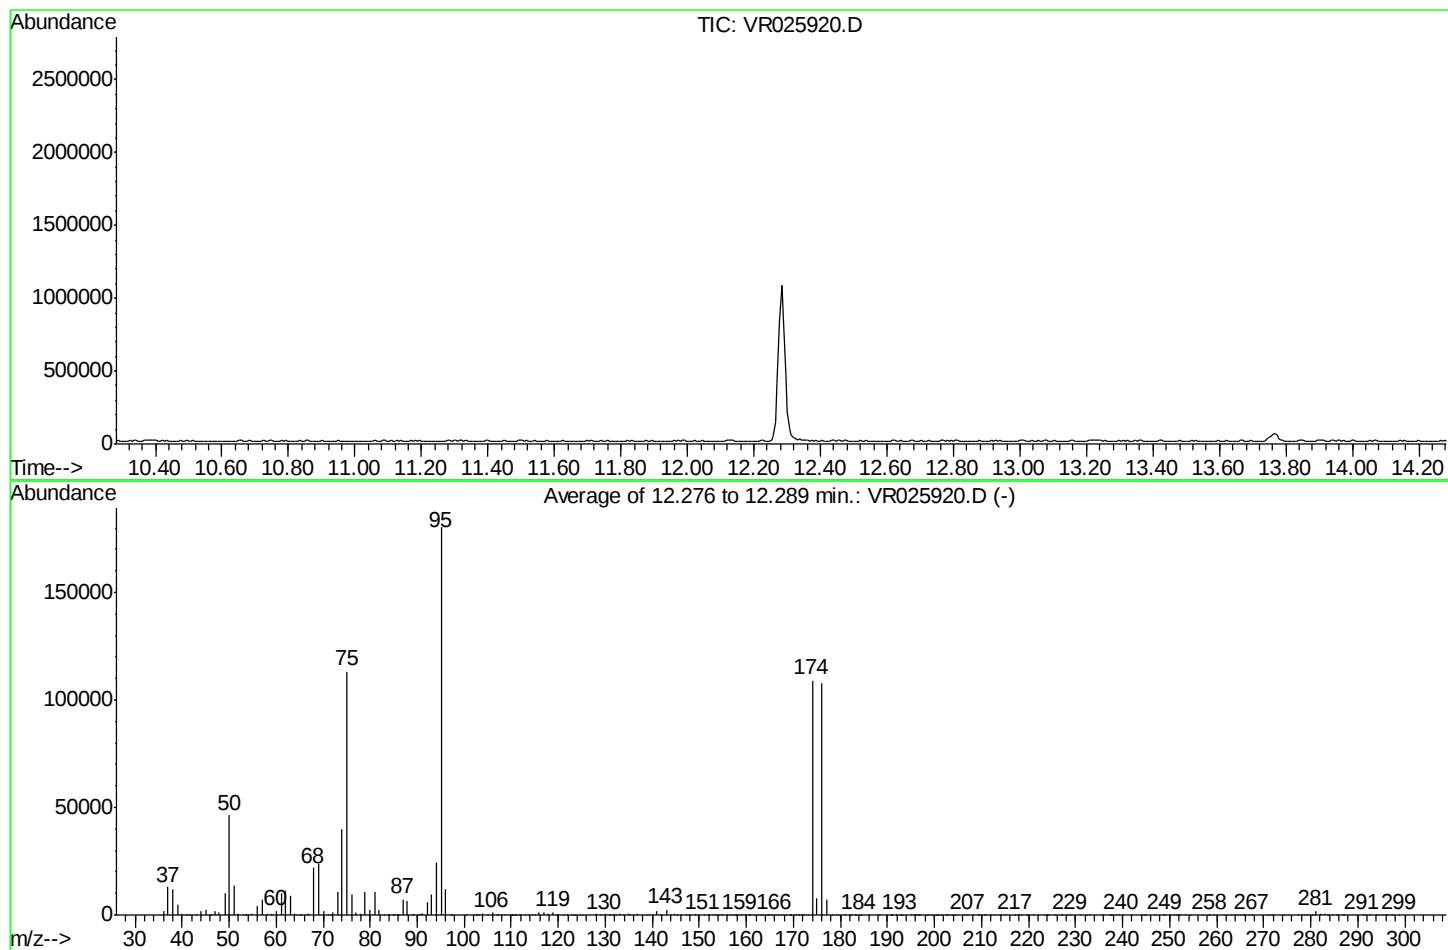

AutoFind: Scans 1742, 1743, 1744; Background Corrected with Scan 1733

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.7	46306	PASS
75	95	30	80	62.8	113245	PASS
95	95	100	100	100.0	180266	PASS
96	95	5	9	6.5	11753	PASS
173	174	0.00	2	0.2	218	PASS
174	95	50	120	60.6	109221	PASS
175	174	5	9	7.1	7773	PASS
176	174	95	101	98.4	107506	PASS
177	176	5	9	6.8	7362	PASS