
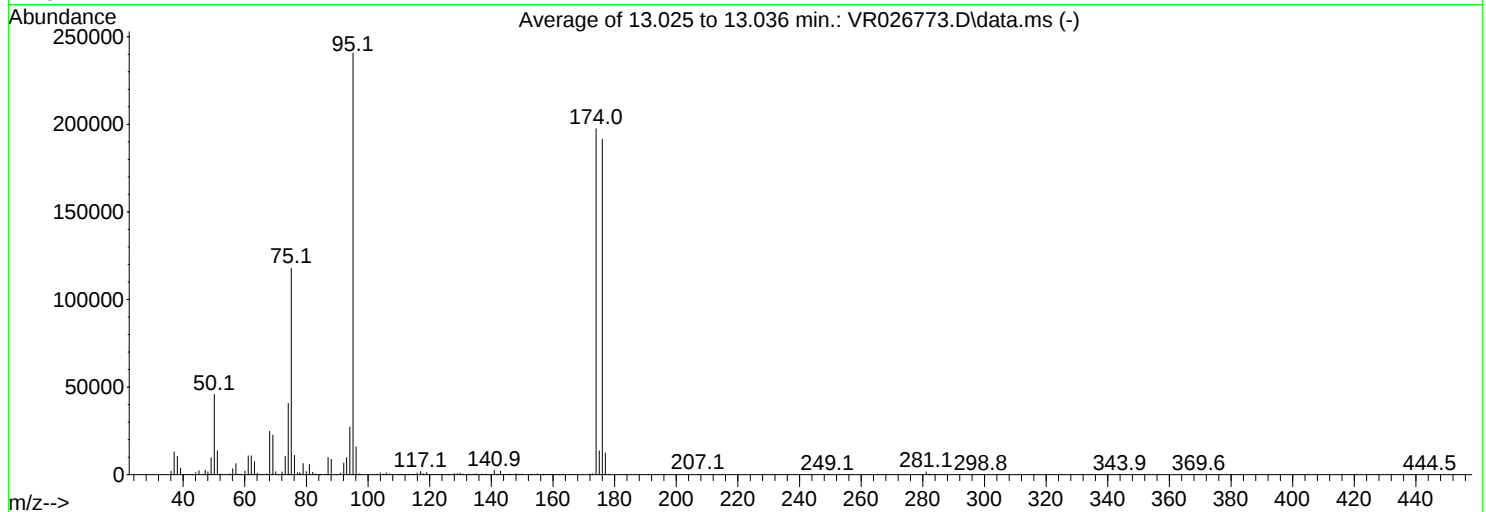


Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR100325\
Data File : VR026773.D
Acq On : 3 Oct 2025 14:07
Operator : SY/MD
Sample : BFB
Misc : 5mL/MSVOA_R/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_T\methods\82R100325W.M
Title : SW846 8260
Last Update : Mon Oct 06 12:35:38 2025

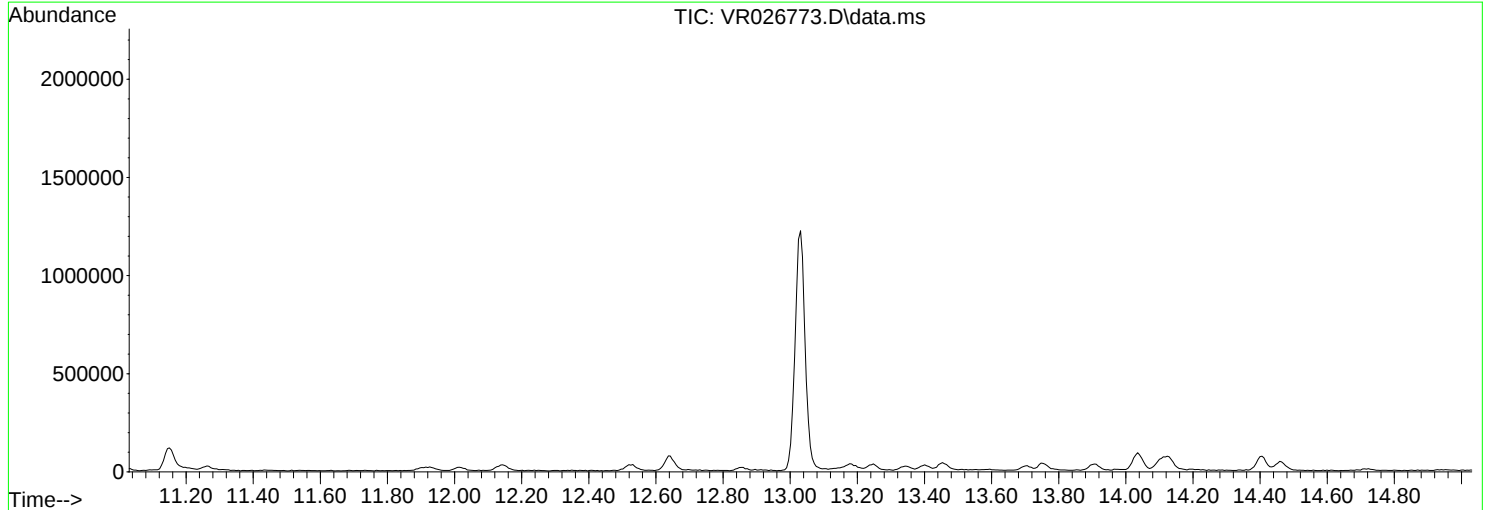

AutoFind: Scans 1948, 1949, 1950; Background Corrected with Scan 1934

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.0	45823	PASS
75	95	30	60	48.9	117819	PASS
95	95	100	100	100.0	240811	PASS
96	95	5	9	6.6	15910	PASS
173	174	0.00	2	0.2	465	PASS
174	95	50	100	82.0	197483	PASS
175	174	5	9	6.9	13620	PASS
176	174	95	101	97.0	191488	PASS
177	176	5	9	6.4	12338	PASS