


Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR100418\
 Data File : VR025942.D
 Acq On : 4 Oct 2018 15:37
 Operator : SY/MD
 Sample : BFB82
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 BFB82

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Oct 05 04:42:35 2018

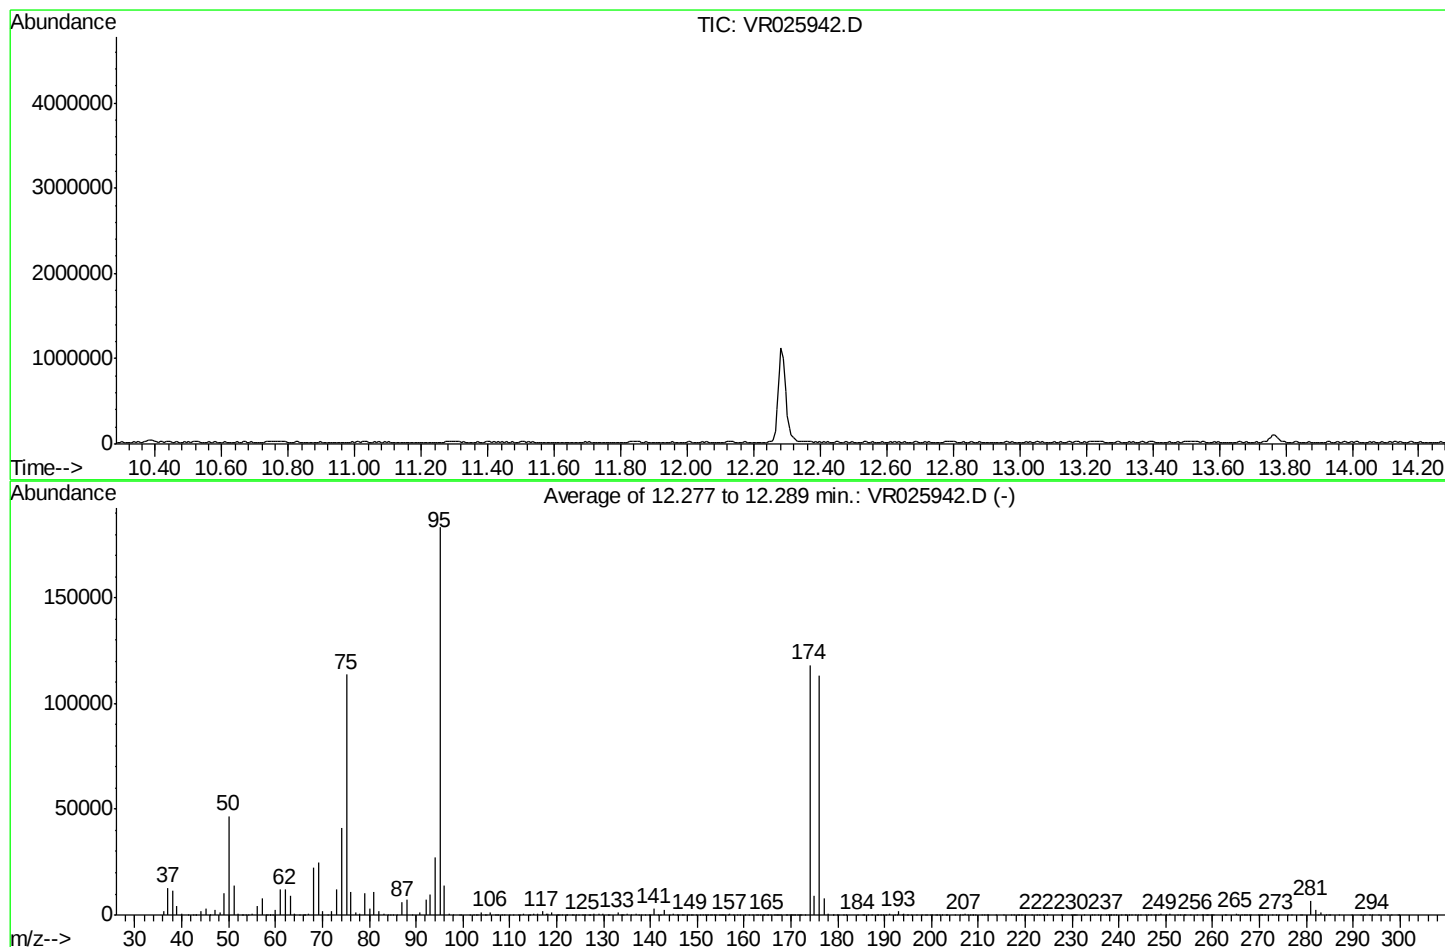

AutoFind: Scans 1742, 1743, 1744; Background Corrected with Scan 1733

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.6	46932	PASS
75	95	30	80	62.0	113664	PASS
95	95	100	100	100.0	183373	PASS
96	95	5	9	7.6	13945	PASS
173	174	0.00	2	0.2	249	PASS
174	95	50	120	64.5	118301	PASS
175	174	5	9	7.5	8906	PASS
176	174	95	101	95.9	113401	PASS
177	176	5	9	6.9	7806	PASS