
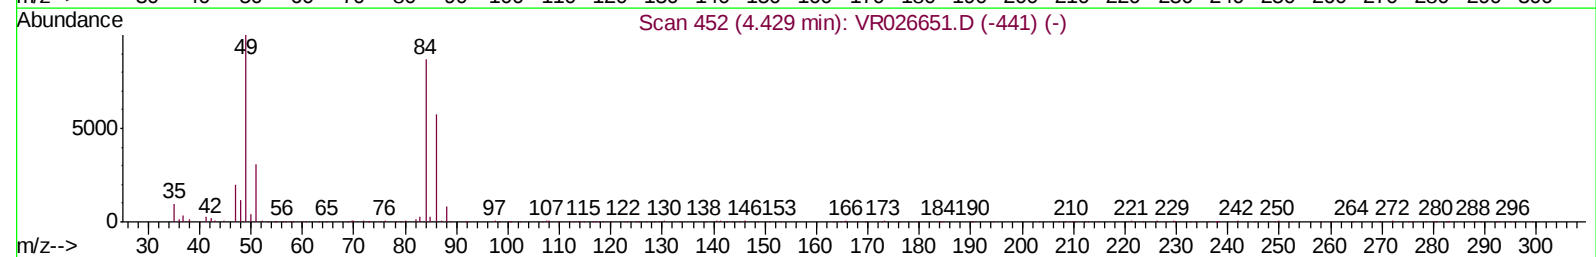
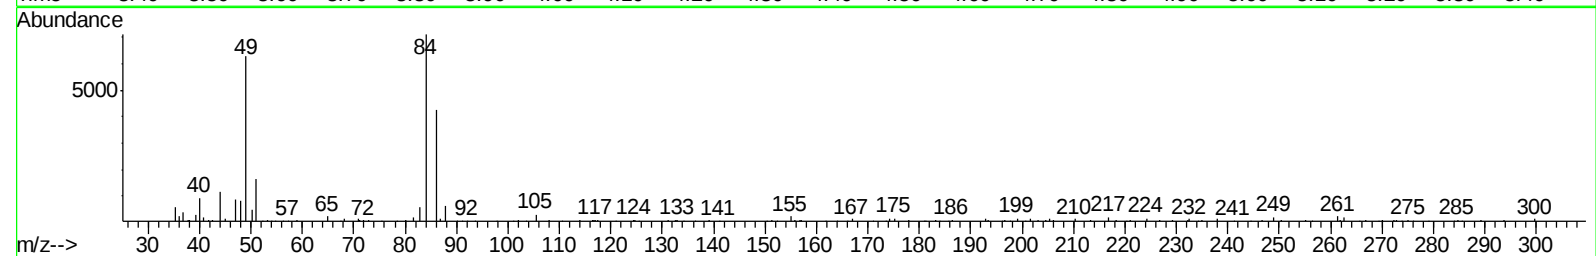


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR101019\
Data File : VR026656.D
Acq On : 10 Oct 2019 18:23
Operator : SY/MD
Sample : VSTD00165
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Oct 11 06:09:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101019WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 11 05:48:01 2019
Response via : Initial Calibration

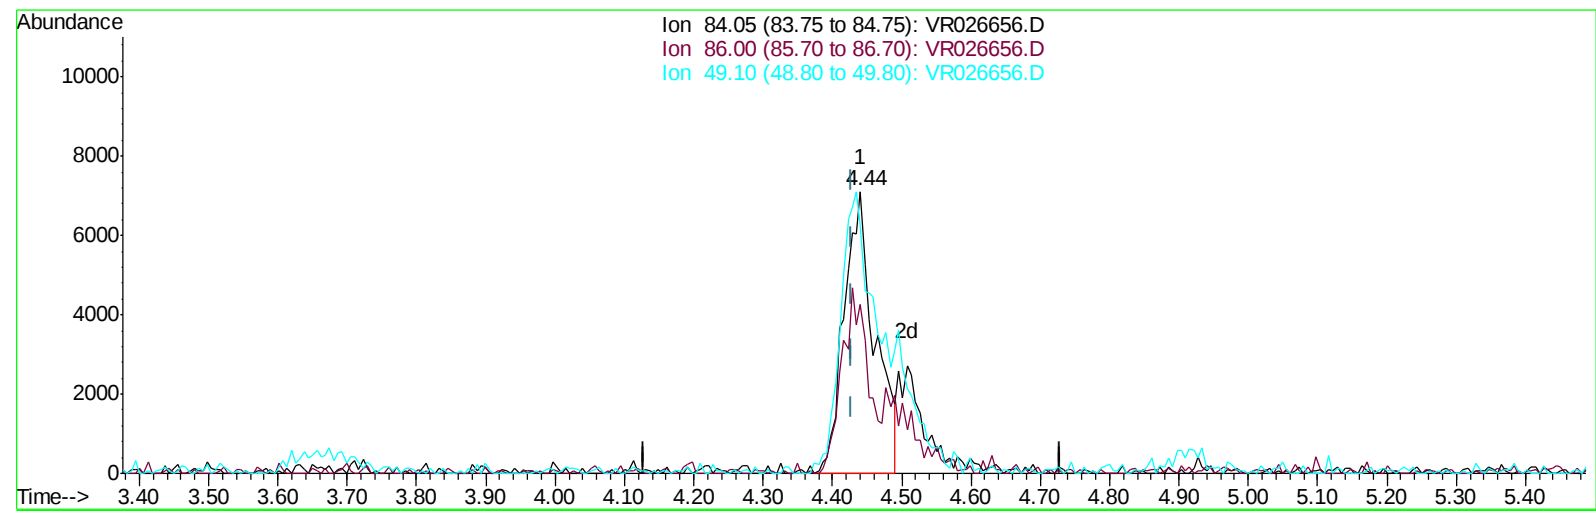

TIC: VR026656.D

(16) Methylene chloride (T)

4.441min (+0.012) 1.13ug/L

response 21875

Ion	Exp%	Act%
84.05	100	100
86.00	66.30	59.93
49.10	115.40	88.28
0.00	0.00	0.00