
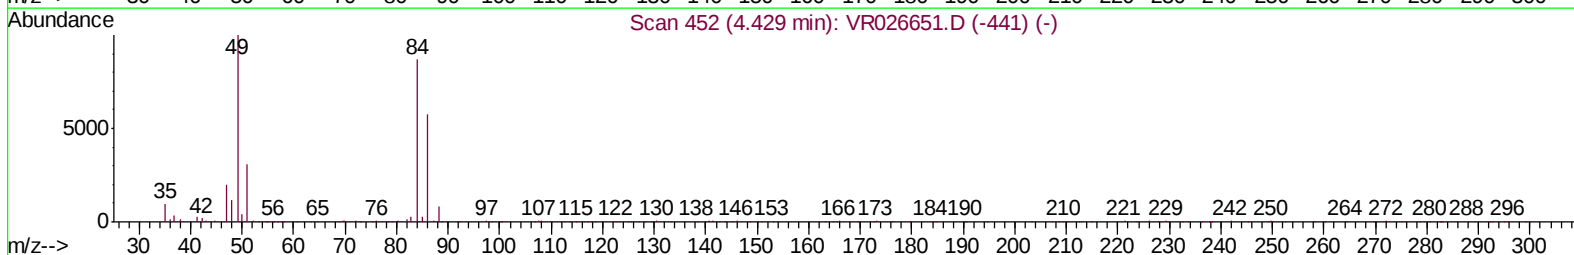
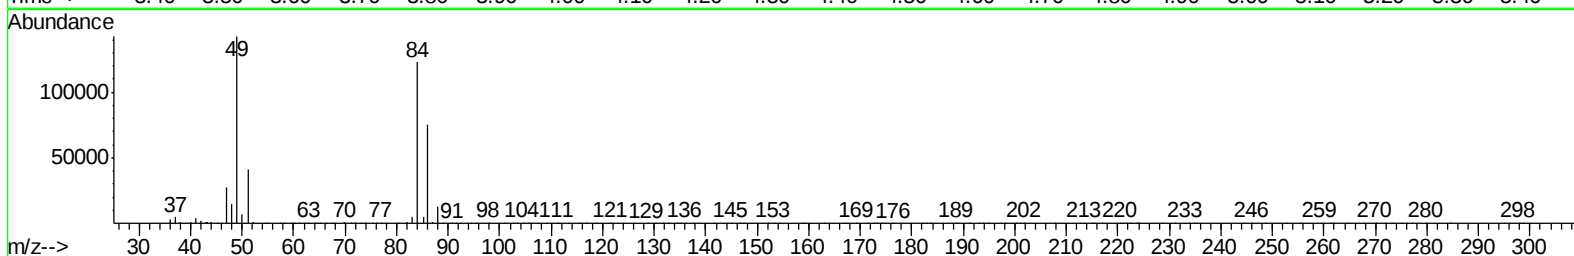


Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_R\DATA\VR101019\  
Data File : VR026653.D  
Acq On : 10 Oct 2019 16:46  
Operator : SY/MD  
Sample : VSTD02068  
Misc : 25mL/MSVOA\_R/WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
MSVOA\_R  
ClientSampleId :

Quant Time: Oct 11 06:08:51 2019  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_R\METHODS\SOMRTR101019WMA.M  
Quant Title : TRACE VOA SOM01.0  
QLast Update : Fri Oct 11 05:48:01 2019  
Response via : Initial Calibration

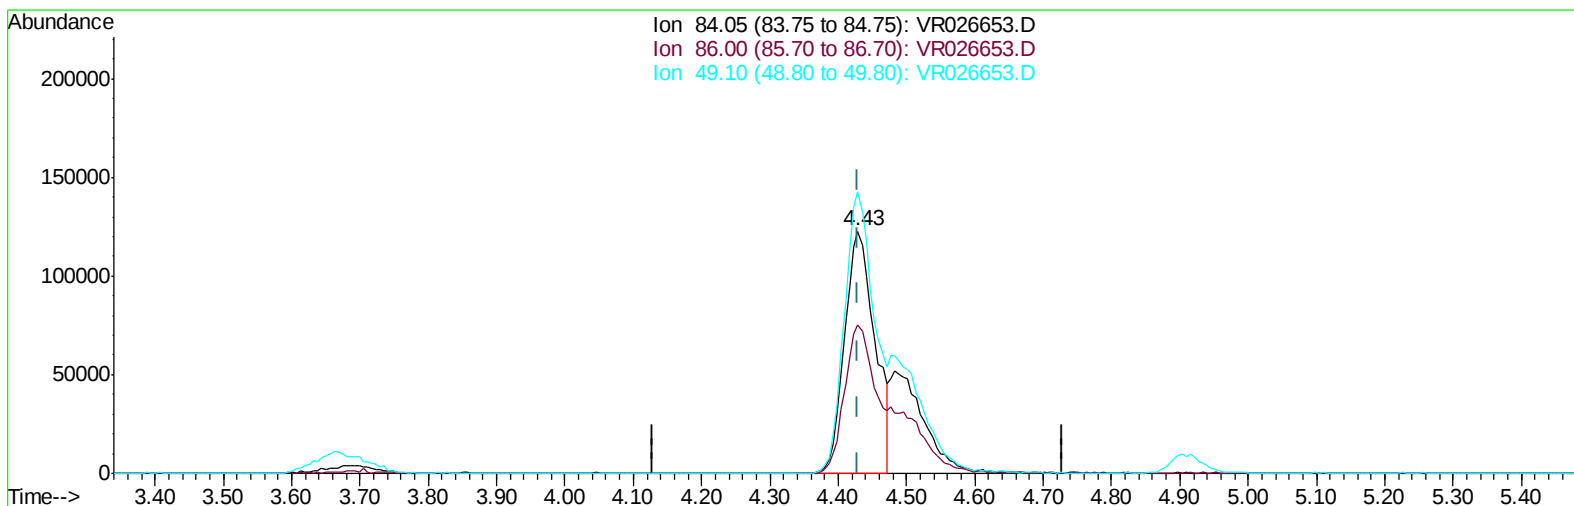

TIC: VR026653.D

(16) Methylene chloride (T)

4.429min (-0.000) 13.85ug/L

response 379241

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 84.05 | 100    | 100    |
| 86.00 | 66.30  | 61.17  |
| 49.10 | 115.40 | 116.21 |
| 0.00  | 0.00   | 0.00   |