
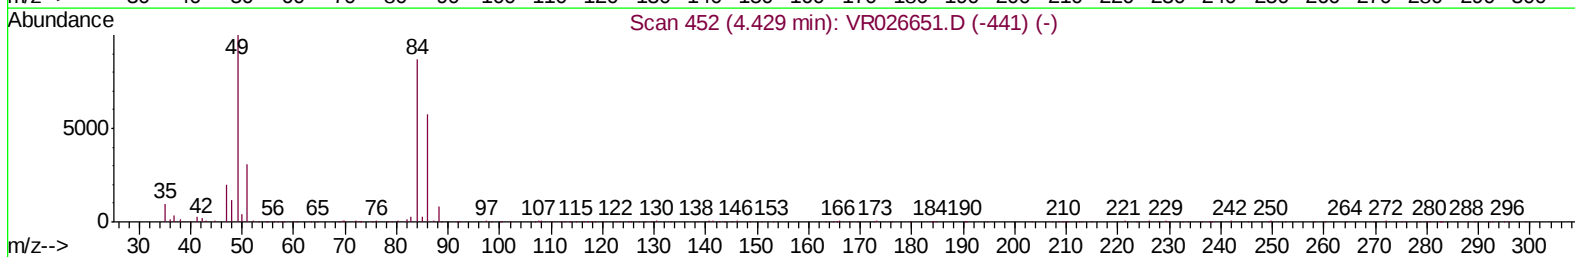
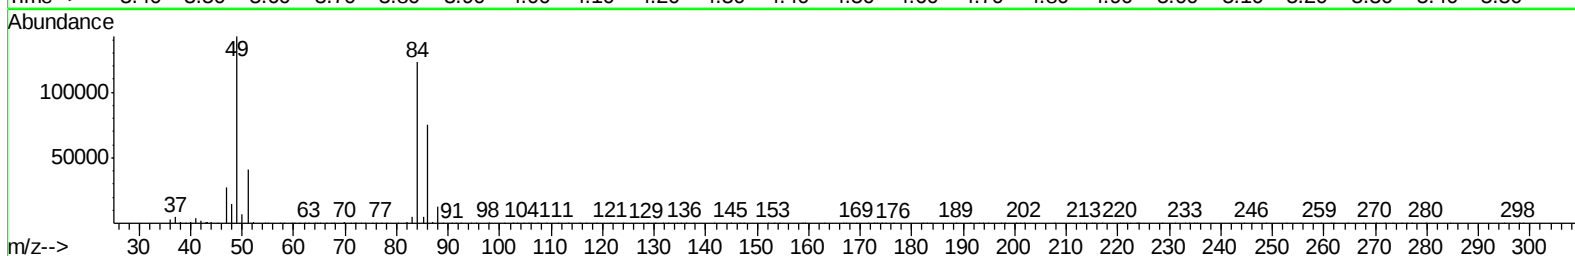


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR101019\
Data File : VR026653.D
Acq On : 10 Oct 2019 16:46
Operator : SY/MD
Sample : VSTD02068
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :

Quant Time: Oct 11 06:08:51 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101019WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 11 05:48:01 2019
Response via : Initial Calibration

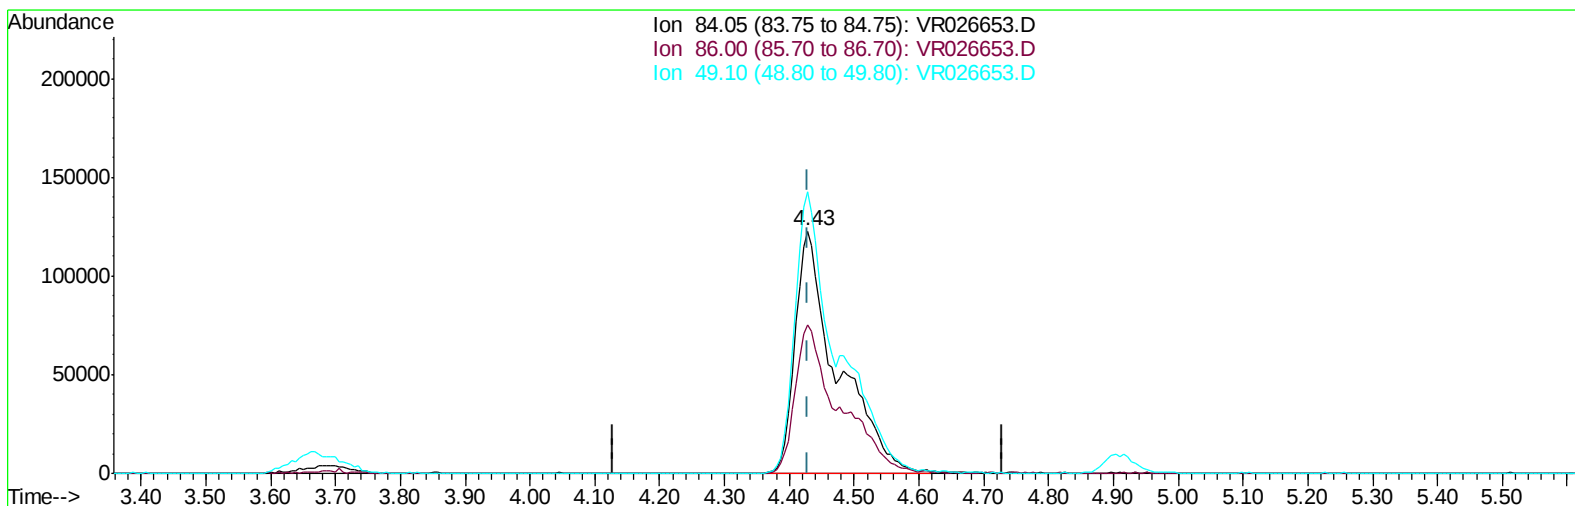

TIC: VR026653.D

(16) Methylene chloride (T)

4.429min (-0.000) 20.28ug/L m

response 555419

Ion	Exp%	Act%
84.05	100	100
86.00	66.30	61.17
49.10	115.40	116.21
0.00	0.00	0.00