
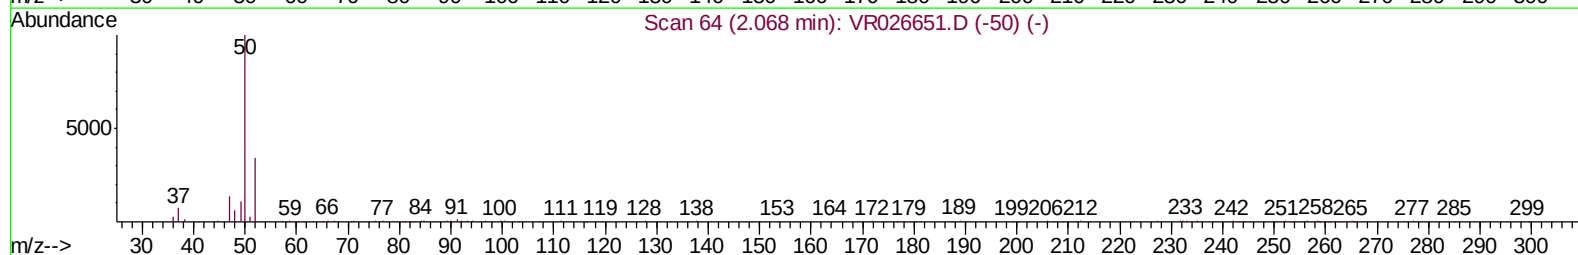
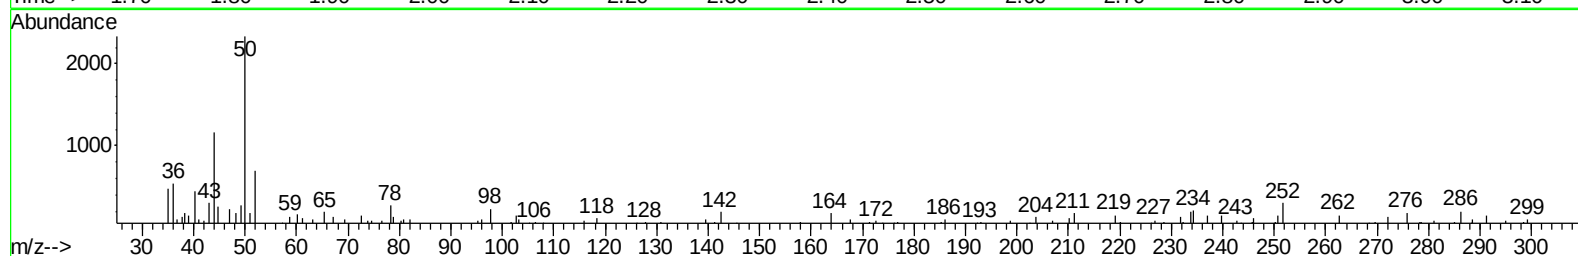


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR101019\
 Data File : VR026655.D
 Acq On : 10 Oct 2019 17:51
 Operator : SY/MD
 Sample : VSTD0.564
 Misc : 25mL/MSVOA_R/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :

Quant Time: Oct 11 06:09:25 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101019WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 11 05:48:01 2019
 Response via : Initial Calibration

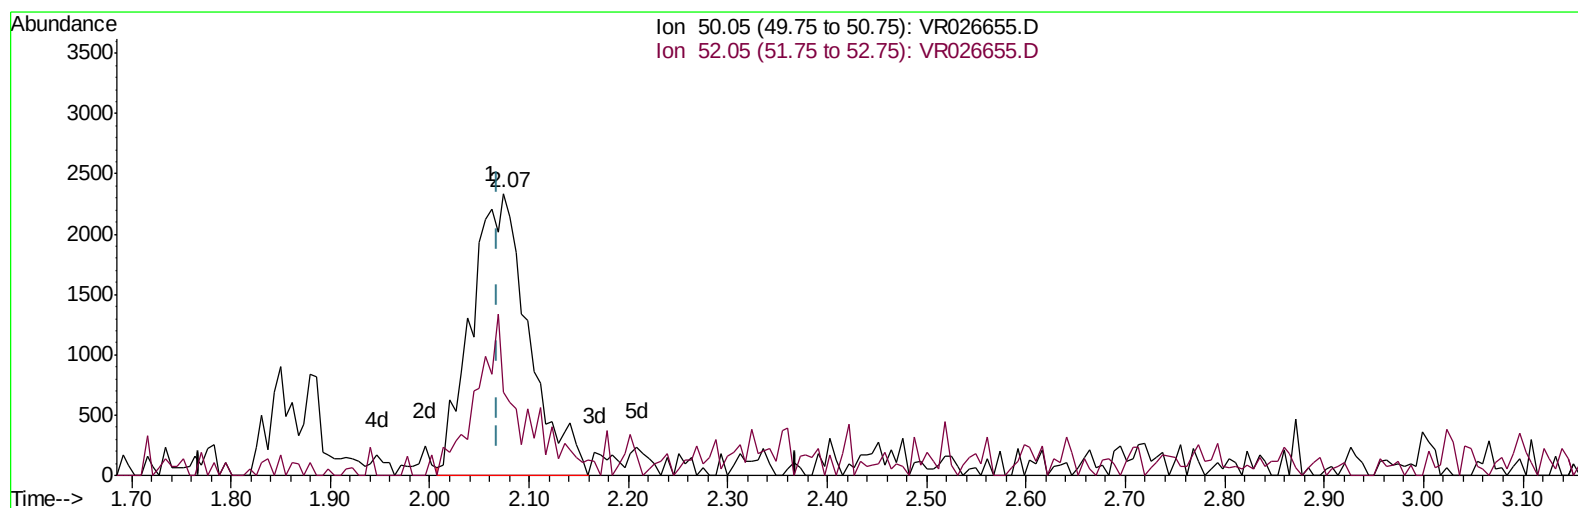

TIC: VR026655.D

(3) Chloromethane (T)

2.074min (+0.006) 0.76ug/L m

response 9383

Ion	Exp%	Act%
50.05	100	100
52.05	34.40	29.59
0.00	0.00	0.00
0.00	0.00	0.00