
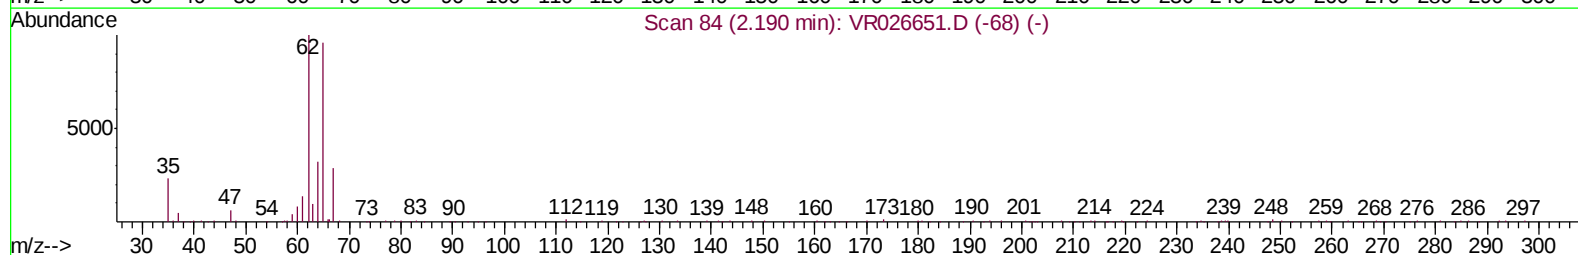
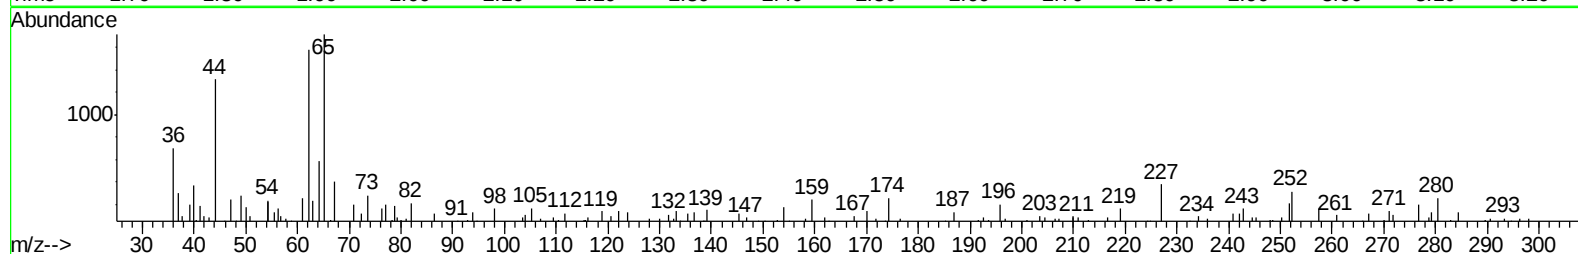


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR101019\
Data File : VR026655.D
Acq On : 10 Oct 2019 17:51
Operator : SY/MD
Sample : VSTD0.564
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :

Quant Time: Oct 11 06:09:25 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101019WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 11 05:48:01 2019
Response via : Initial Calibration

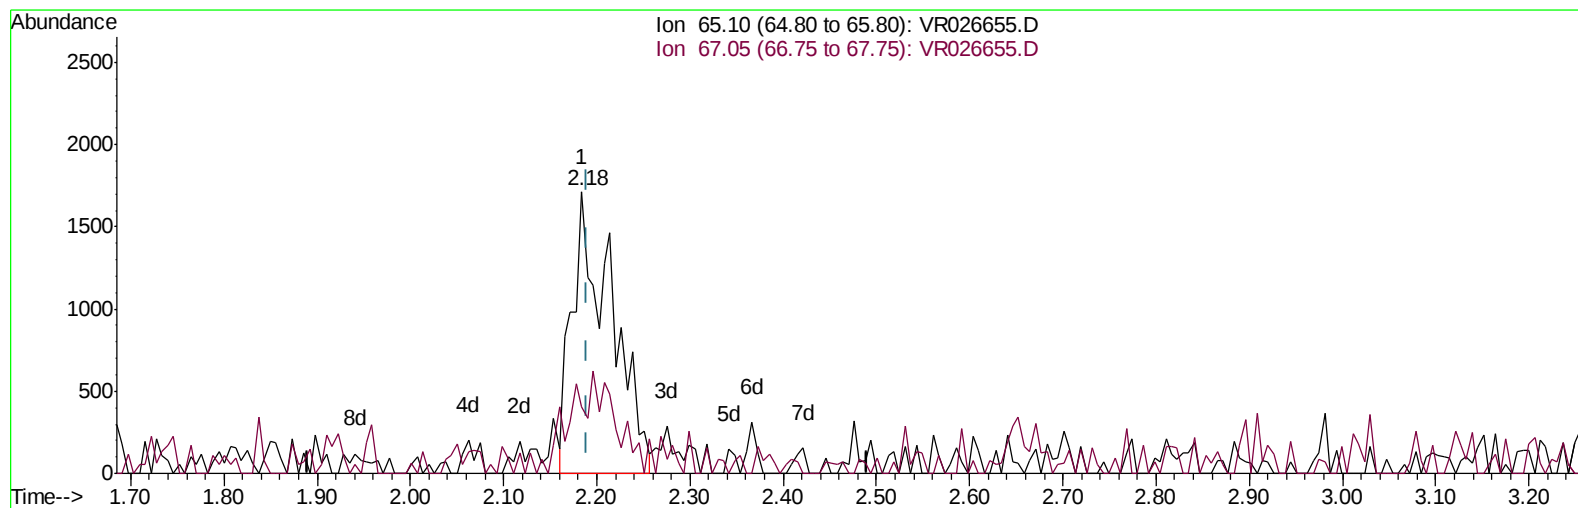

TIC: VR026655.D

(4) Vinyl Chloride-d3 (S)

2.184min (-0.006) 0.76ug/L m

response 5057

Ion	Exp%	Act%
65.10	100	100
67.05	32.40	17.78#
0.00	0.00	0.00
0.00	0.00	0.00