

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR101118\
 Data File : VR026046.D
 Acq On : 11 Oct 2018 15:49
 Operator : SY/MD
 Sample : J5315-13
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 C0JA4

Quant Time: Oct 12 08:50:23 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 12 08:06:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	443868	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	387873	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	128934	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.15	65	130565	3.73	ug/L	-0.01
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.60%
7) Chloroethane-d5	2.63	69	128995	4.51	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.20%
11) 1,1-Dichloroethene-d2	3.63	63	241431	2.94	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.80%#
20) 2-Butanone-d5	6.59	46	244198	62.58	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	125.16%
24) Chloroform-d	7.20	84	279338	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.60%
26) 1,2-Dichloroethane-d4	7.90	65	132807	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.40%
32) Benzene-d6	7.85	84	505603	3.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.40%
36) 1,2-Dichloropropane-d6	8.90	67	156325	4.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.80%
41) Toluene-d8	9.97	98	435331	3.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.80%
43) trans-1,3-Dichloropropene-	10.24	79	33843	4.29	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.80%
46) 2-Hexanone-d5	10.59	63	188114	62.47	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	124.94%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	74615	5.29	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.80%
64) 1,2-Dichlorobenzene-d4	13.51	152	100560	4.87	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.40%


Target Compounds					Ovalue
13) Acetone	3.70	43	8389	2.966 ug/L	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR101118\
Data File : VR026046.D
Acq On : 11 Oct 2018 15:49
Operator : SY/MD
Sample : J5315-13
Misc : 25mL/MSVOA R/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
C0JA4

Quant Time: Oct 12 08:50:23 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 12 08:06:28 2018
Response via : Initial Calibration

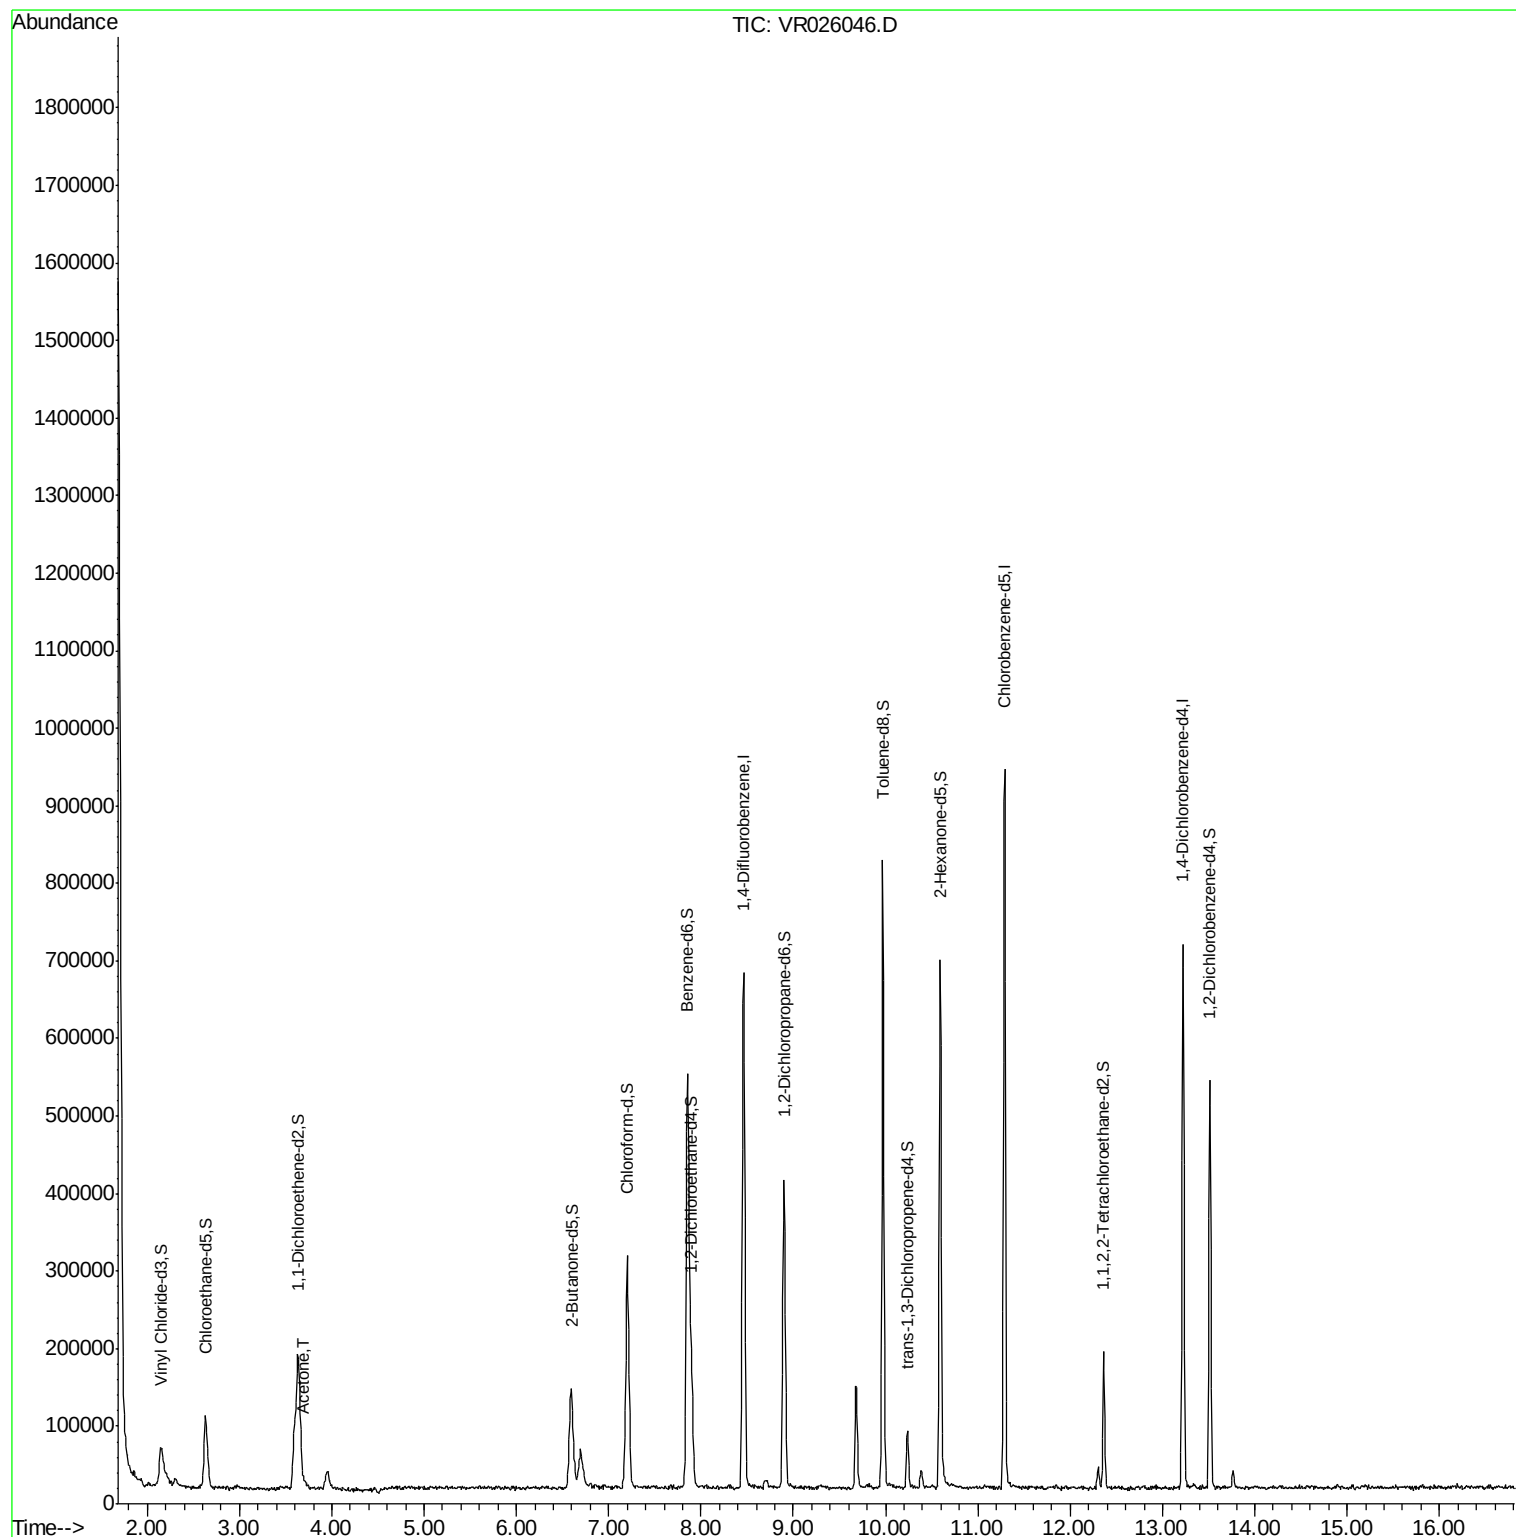

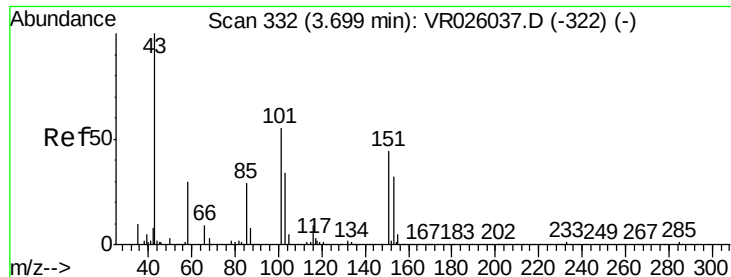

#13

Acetone

Concen: 2.966 ug/L

RT: 3.70 min Scan# 332

Delta R.T. -0.00 min

Lab File: VR026046.D

Acq: 11 Oct 2018 15:49

Instrument :
MSVOA_R
ClientSampleId :
C0JA4

Tot Ion: 43 Resp: 8389

Ion Ratio Lower Upper

43 100

58 36.3 0.0 51.4

