

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR101518\
 Data File : VR026084.D
 Acq On : 15 Oct 2018 21:49
 Operator : SY/MD
 Sample : J5379-02
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :

Quant Time: Oct 16 08:25:11 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 16 08:21:47 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	564271	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	481982	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	154747	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.15	65	243982	4.94	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.80%
7) Chloroethane-d5	2.63	69	217306	5.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.40%
11) 1,1-Dichloroethene-d2	3.61	63	467187	3.85	ug/L	-0.02
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.00%
20) 2-Butanone-d5	6.59	46	231259	57.04	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.08%
24) Chloroform-d	7.20	84	374615	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.40%
26) 1,2-Dichloroethane-d4	7.90	65	160725	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.40%
32) Benzene-d6	7.85	84	747796	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.60%
36) 1,2-Dichloropropane-d6	8.90	67	212182	5.31	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.20%
41) Toluene-d8	9.97	98	695514	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.20%
43) trans-1,3-Dichloropropene-	10.24	79	50086	4.78	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.60%
46) 2-Hexanone-d5	10.59	63	180250	59.52	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	119.04%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	76932	4.90	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.00%
64) 1,2-Dichlorobenzene-d4	13.52	152	124981	5.11	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.20%

Target Compounds

					Ovalue
3) Chloromethane	2.02	50	10565	0.176 ug/L #	81
12) 1,1-Dichloroethene	3.63	96	5771	0.105 ug/L #	1
13) Acetone	3.70	43	10976	2.619 ug/L	80
18) trans-1,2-Dichloroethene	4.88	96	17284	0.417 ug/L	87
19) 1,1-Dichloroethane	5.69	63	35204	0.452 ug/L	93
22) cis-1,2-Dichloroethene	6.67	96	5345207	136.174 ug/L #	87
25) Chloroform	7.24	83	59002	0.776 ug/L	92
29) 1,1,1-Trichloroethane	7.43	97	45181	0.686 ug/L	93
34) Trichloroethene	8.71	95	13860473	299.431 ug/L	82
35) Methylcyclohexane	8.90	83	50295	0.730 ug/L #	17
37) 1,2-Dichloropropane	8.90	63	26237	0.688 ug/L #	93
44) trans-1,3-Dichloropropene	10.24	75	3294	0.108 ug/L	85
45) 1,1,2-Trichloroethane	10.45	97	8809	0.547 ug/L	94
47) Tetrachloroethene	10.51	164	65466	1.981 ug/L	99
48) 2-Hexanone	10.59	43	27374	3.597 ug/L #	71
49) Dibromochloromethane	10.51	129	54238	2.995 ug/L #	11

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR101518\
Data File : VR026084.D
Acq On : 15 Oct 2018 21:49
Operator : SY/MD
Sample : J5379-02
Misc : 25mL/MSVOA R/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :

Quant Time: Oct 16 08:25:11 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 16 08:21:47 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR101518\
Data File : VR026084.D
Acq On : 15 Oct 2018 21:49
Operator : SY/MD
Sample : J5379-02
Misc : 25mL/MSVOA R/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :

Quant Time: Oct 16 08:25:11 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 16 08:21:47 2018
Response via : Initial Calibration




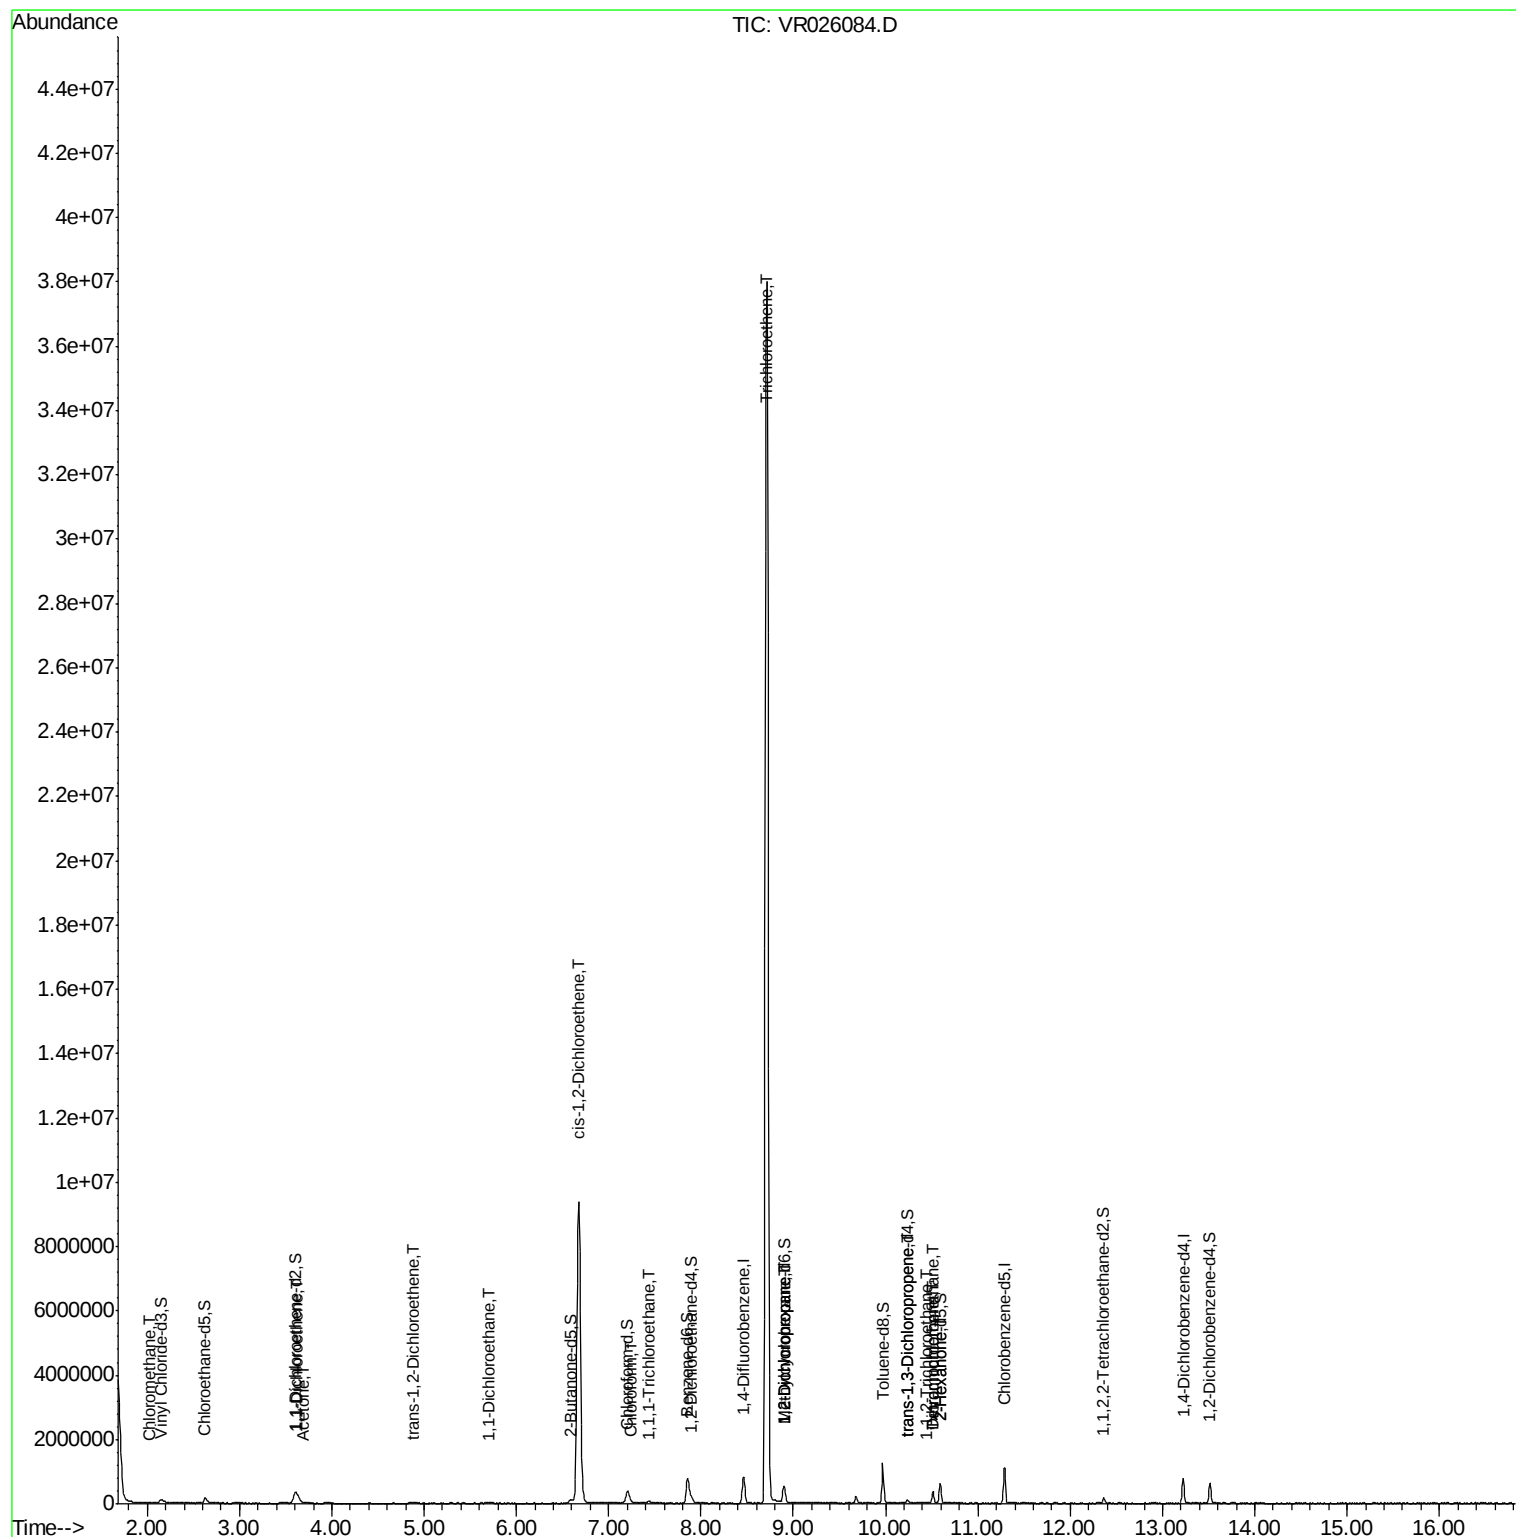


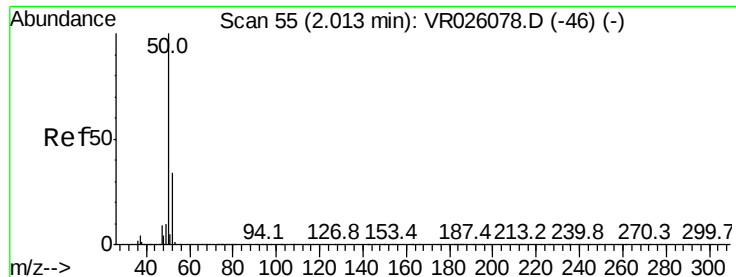

#3
Chloromethane
Concen: 0.176 ug/L
RT: 2.02 min Scan# 56
Delta R.T. 0.01 min
Lab File: VR026084.D
Acq: 15 Oct 2018 21:49




Instrument :
MSVOA_R
ClientSampleId :


Tot Ion: 50 Resp: 10565
Ion Ratio Lower Upper
50 100
52 42.0 22.0 40.8#

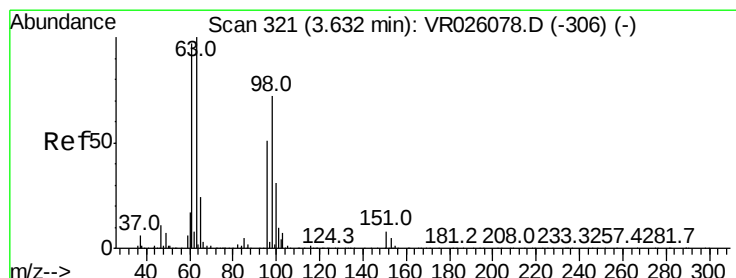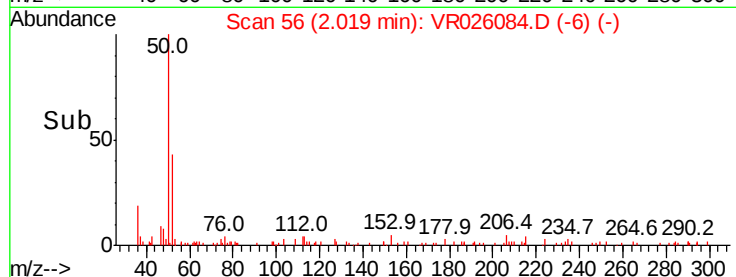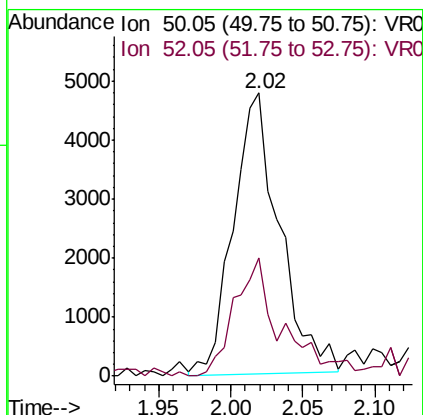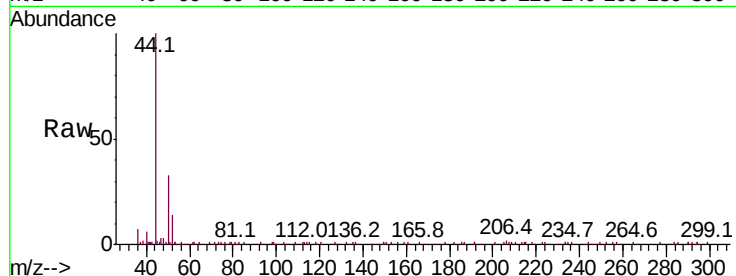

#12
1,1-Dichloroethene
Concen: 0.105 ug/L
RT: 3.63 min Scan# 320
Delta R.T. -0.01 min
Lab File: VR026084.D
Acq: 15 Oct 2018 21:49

Tgt Ion: 96 Resp: 5771
Ion Ratio Lower Upper
96 100
61 639.4 126.7 235.3#
63 3811.6 125.0 232.2#

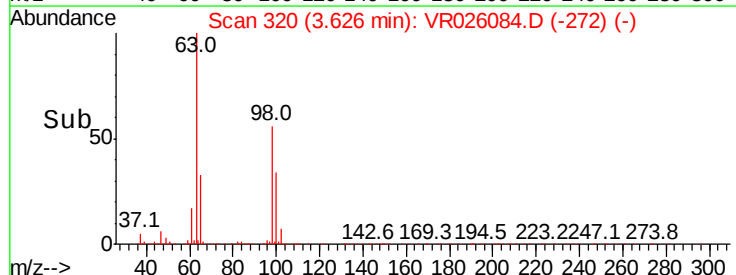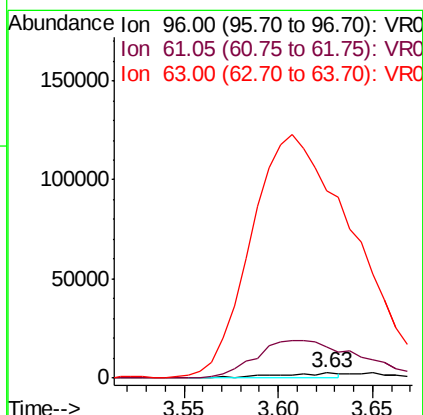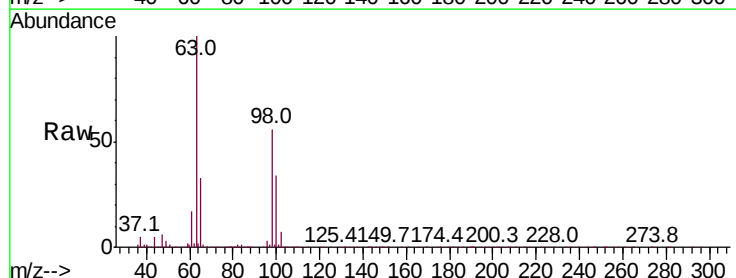

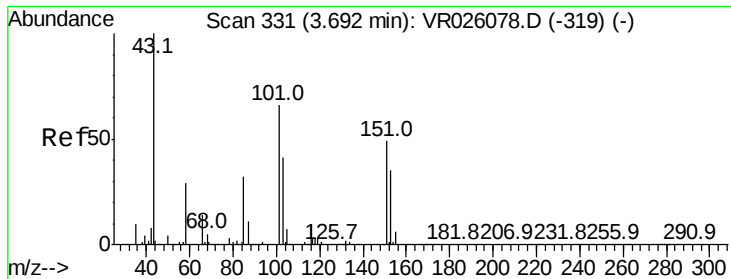

#13

Acetone

Concen: 2.619 ug/L

RT: 3.70 min Scan# 332

Delta R.T. 0.01 min

Lab File: VR026084.D

Acq: 15 Oct 2018 21:49





Instrument :
MSVOA_R
ClientSampled :

Tot Ion: 43 Resp: 10976

Ion Ratio Lower Upper

43 100

58 17.4 0.0 55.4

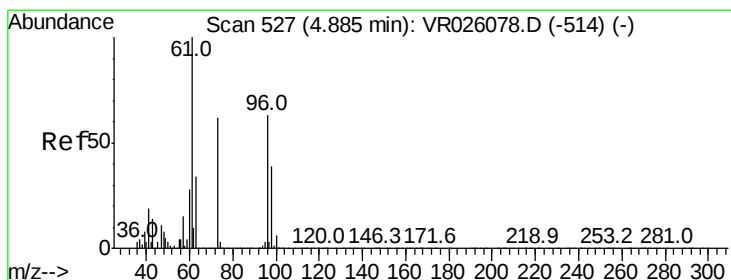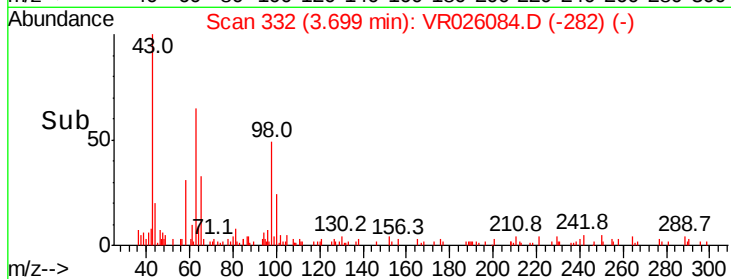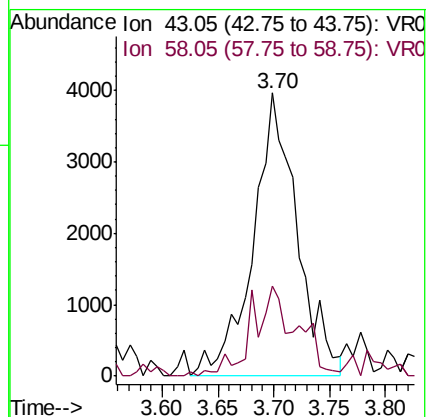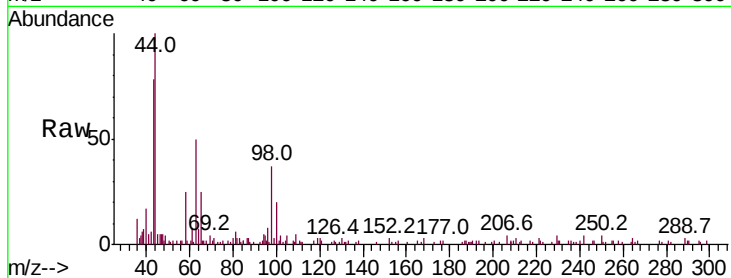

#18

trans-1,2-Dichloroethene

Concen: 0.417 ug/L

RT: 4.88 min Scan# 527

Delta R.T. 0.00 min

Lab File: VR026084.D

Acq: 15 Oct 2018 21:49




Tgt Ion: 96 Resp: 17284


Ion Ratio Lower Upper

96 100

61 137.2 111.4 206.8

98 61.7 41.4 77.0

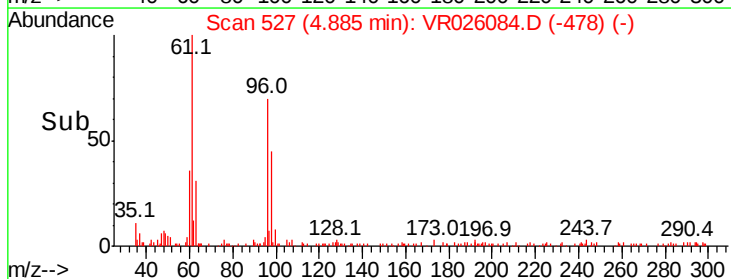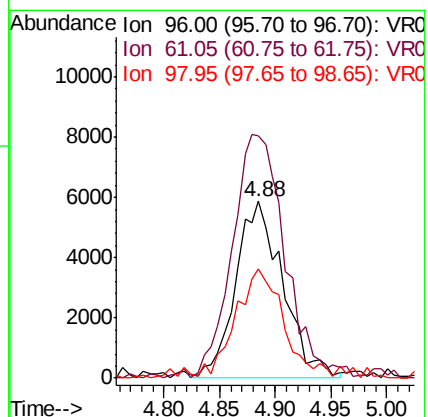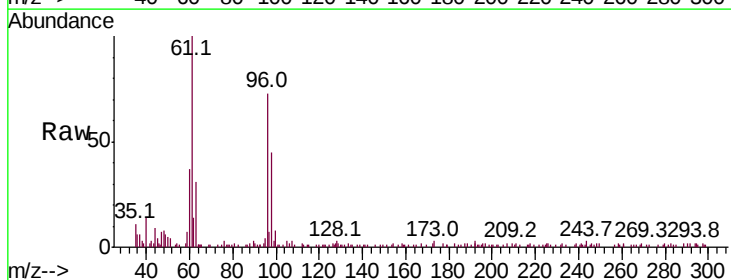

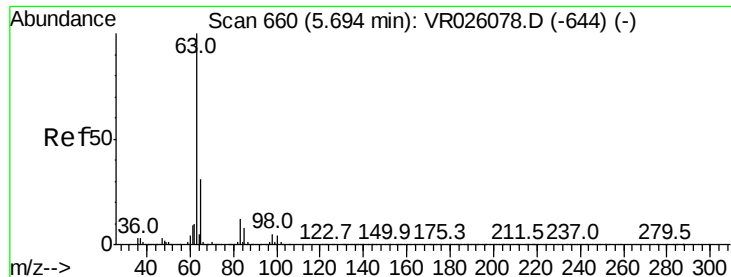

#19

1,1-Dichloroethane

Concen: 0.452 ug/L

RT: 5.69 min Scan# 660

Delta R.T. 0.00 min

Lab File: VR026084.D

Acq: 15 Oct 2018 21:49

Instrument :
MSVOA_R
ClientSampleId :


Tot Ion: 63 Resp: 35204

Ion	Ratio	Lower	Upper
63	100		
65	26.5	21.2	39.4
83	15.6	9.2	17.2

63 100

65 26.5 21.2 39.4




83 15.6 9.2 17.2

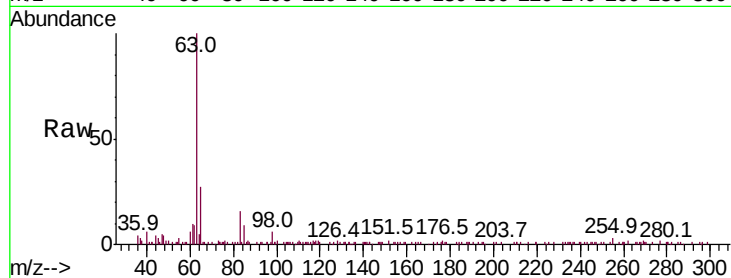

Abundance Ion 63.10 (62.80 to 63.80): VR0

Ion 65.10 (64.80 to 65.80): VR0

Ion 83.05 (82.75 to 83.75): VR0

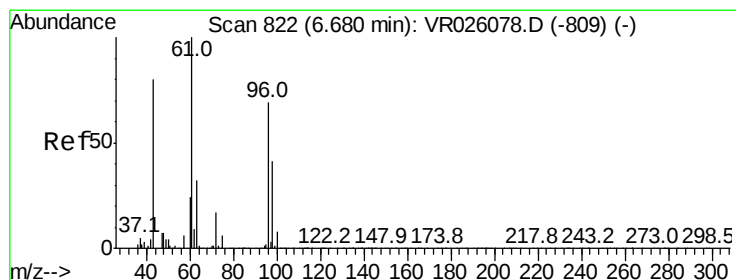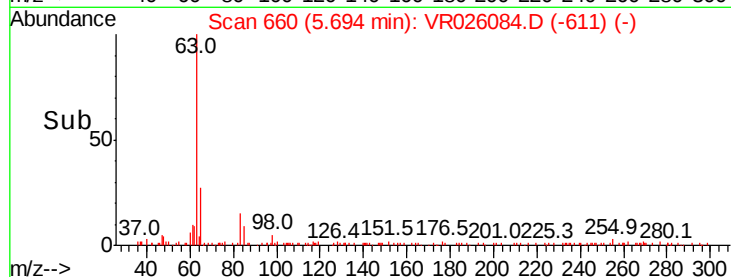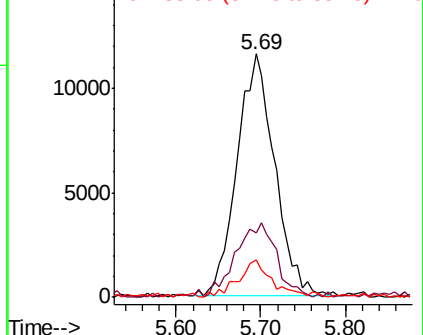

#22

cis-1,2-Dichloroethene

Concen: 136.174 ug/L

RT: 6.67 min Scan# 821

Delta R.T. -0.01 min

Lab File: VR026084.D

Acq: 15 Oct 2018 21:49


Tgt Ion: 96 Resp: 5345207

Ion	Ratio	Lower	Upper
96	100		
61	128.8	101.8	189.0
68	0.0	0.1	0.3#

96 100

61 128.8 101.8 189.0



68 0.0 0.1 0.3#

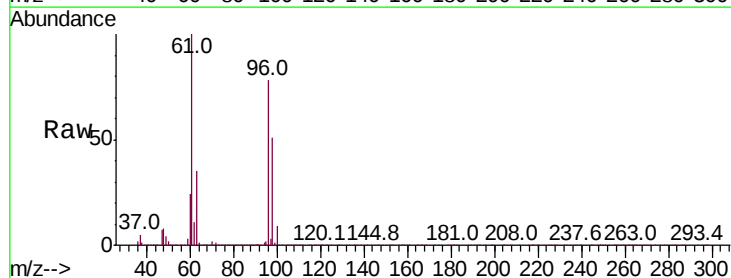


Abundance Ion 96.00 (95.70 to 96.70): VR0

Ion 61.05 (60.75 to 61.75): VR0

Ion 68.15 (67.85 to 68.85): VR0



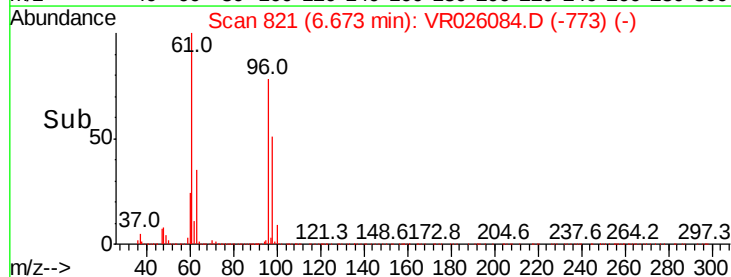
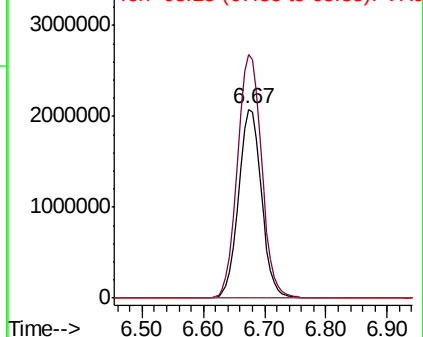


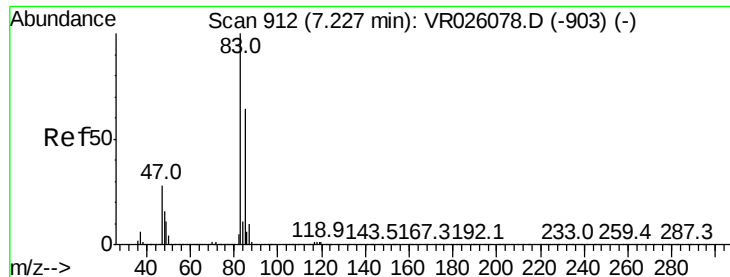

#25
Chloroform
Concen: 0.776 ug/L
RT: 7.24 min Scan# 914
Delta R.T. 0.01 min
Lab File: VR026084.D
Acq: 15 Oct 2018 21:49




Instrument :
MSVOA_R
ClientSampled :


Tot Ion: 83 Resp: 59002
Ion Ratio Lower Upper
83 100
85 68.0 43.5 80.7

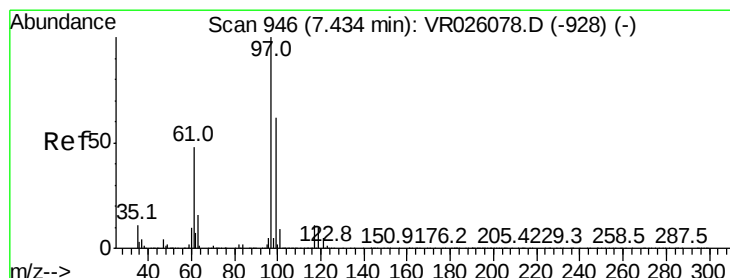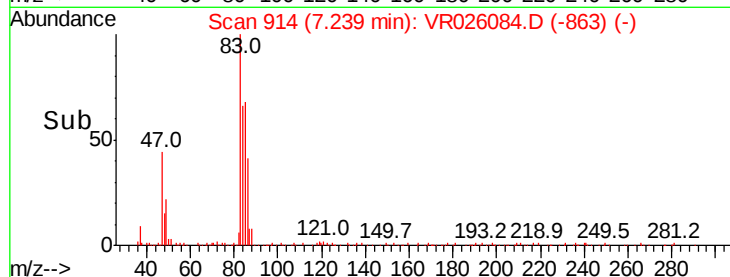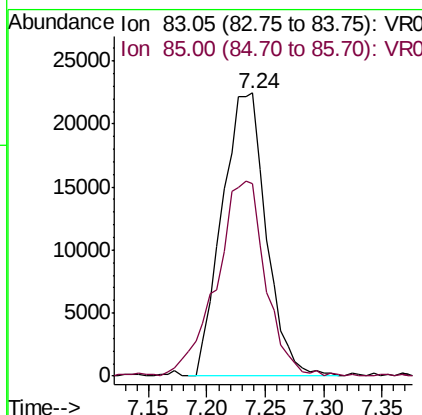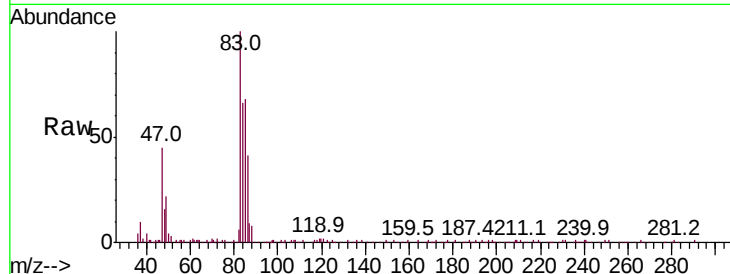

#29
1,1,1-Trichloroethane
Concen: 0.686 ug/L
RT: 7.43 min Scan# 946
Delta R.T. 0.00 min
Lab File: VR026084.D
Acq: 15 Oct 2018 21:49

Tgt Ion: 97 Resp: 45181
Ion Ratio Lower Upper
97 100
99 65.9 51.1 76.7
61 61.0 42.1 63.1

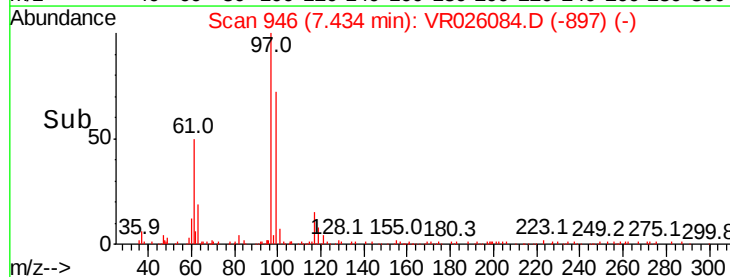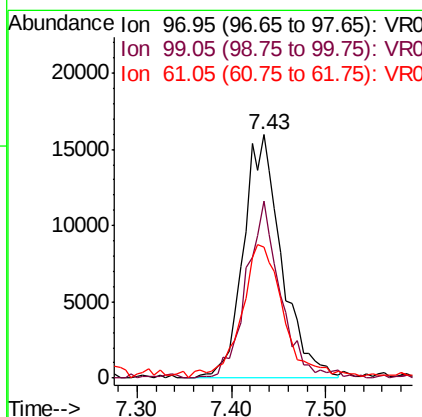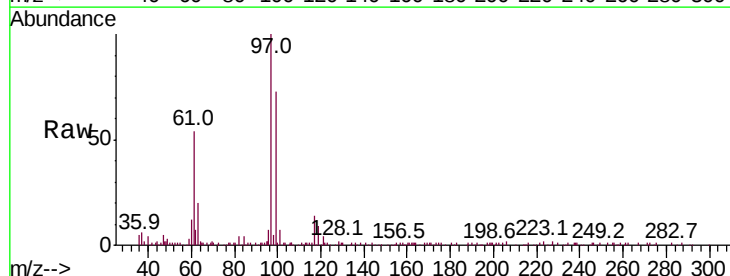

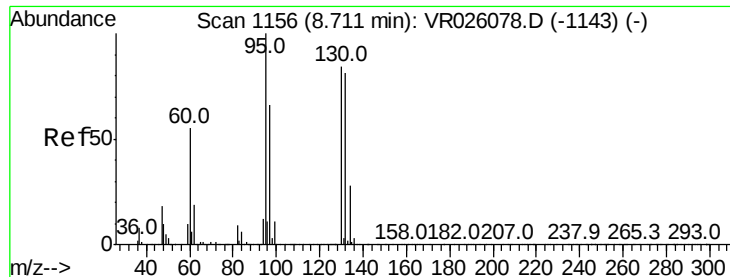

#34

Trichloroethene

Concen: 299.431 ug/L

RT: 8.71 min Scan# 1156

Delta R.T. 0.00 min

Lab File: VR026084.D

Acq: 15 Oct 2018 21:49

Instrument :
MSVOA_R
ClientSampleId :

Tot Ion: 95 Resp:13860473


Ion Ratio Lower Upper

95 100

97 81.8 45.7 84.9

132 102.3 58.3 108.3

130 103.7 64.0 119.0



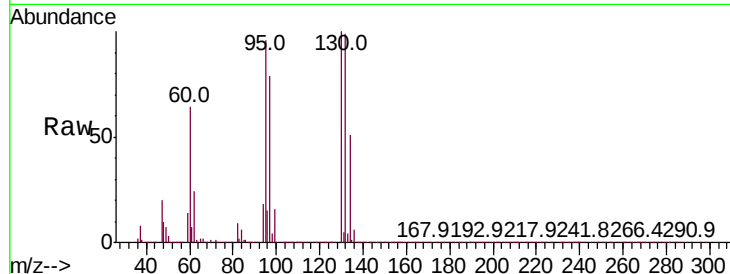


Abundance Ion 95.00 (94.70 to 95.70): VR0

Ion 96.95 (96.65 to 97.65): VR0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

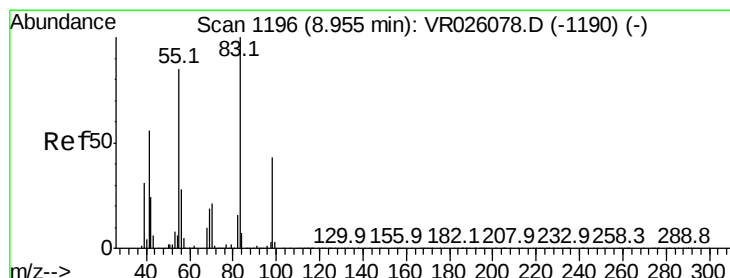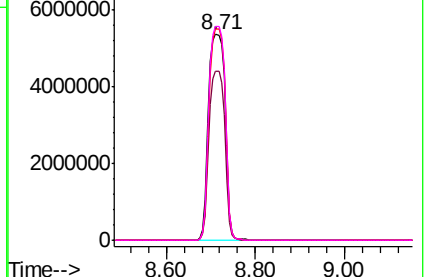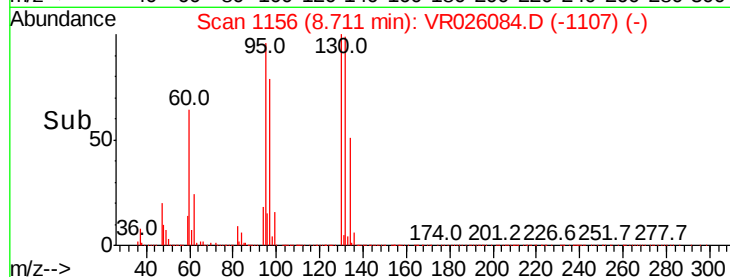

#35

Methylcyclohexane

Concen: 0.730 ug/L

RT: 8.90 min Scan# 1187

Delta R.T. -0.05 min

Lab File: VR026084.D

Acq: 15 Oct 2018 21:49


Tgt Ion: 83 Resp: 50295

Ion Ratio Lower Upper

83 100

55 2.1 66.8 100.2#



98 0.0 35.2 52.8#

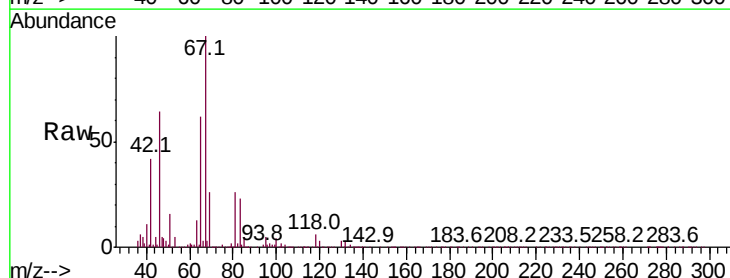


Abundance Ion 83.15 (82.85 to 83.85): VR0

Ion 55.10 (54.80 to 55.80): VR0

Ion 98.15 (97.85 to 98.85): VR0

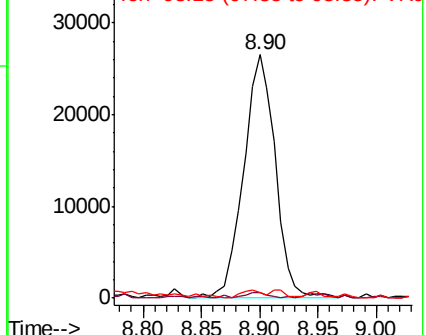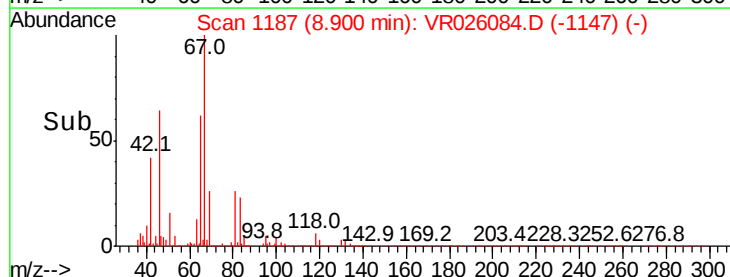

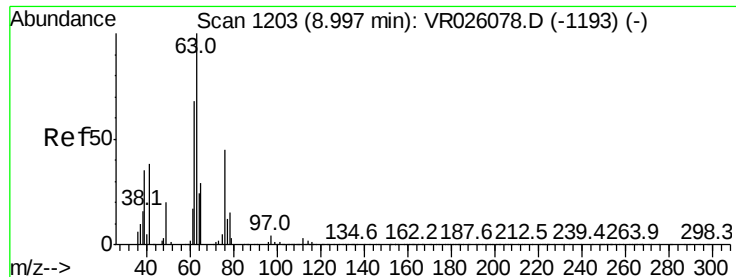

#37

1,2-Dichloropropane

Concen: 0.688 ug/L

RT: 8.90 min Scan# 1187





Delta R.T. -0.10 min

Lab File: VR026084.D

Acq: 15 Oct 2018 21:49

Instrument :
MSVOA_R
ClientSampleId :

Tot Ion: 63 Resp: 26237
Ion Ratio Lower Upper
63 100
112 1.0 2.7 4.1#

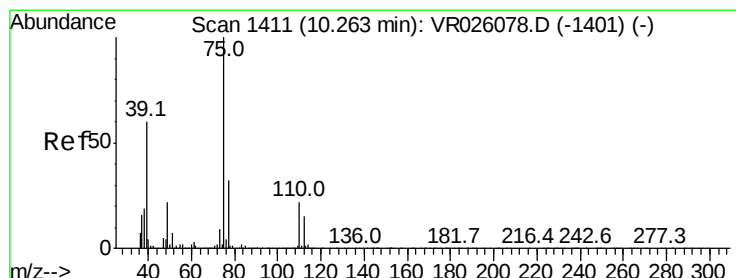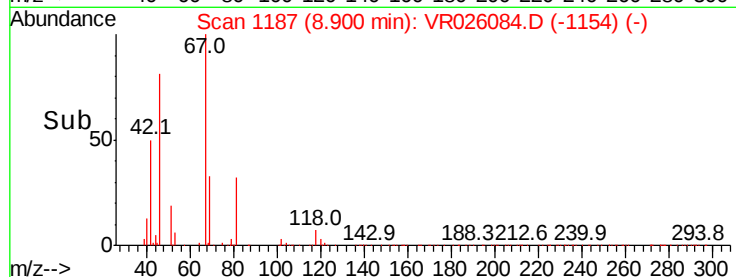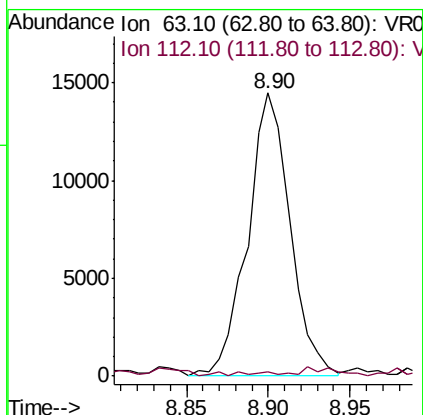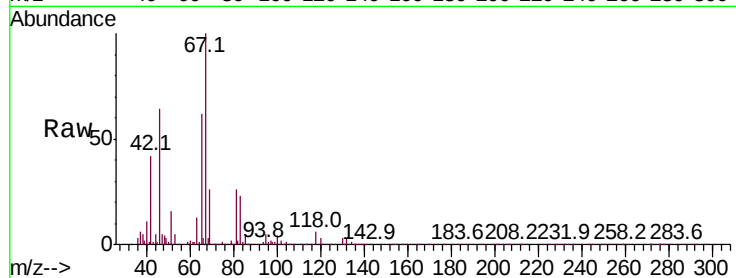

#44

trans-1,3-Dichloropropene

Concen: 0.108 ug/L




RT: 10.24 min Scan# 1407


Delta R.T. -0.02 min

Lab File: VR026084.D

Acq: 15 Oct 2018 21:49

Tgt Ion: 75 Resp: 3294
Ion Ratio Lower Upper
75 100
77 25.7 24.1 44.7


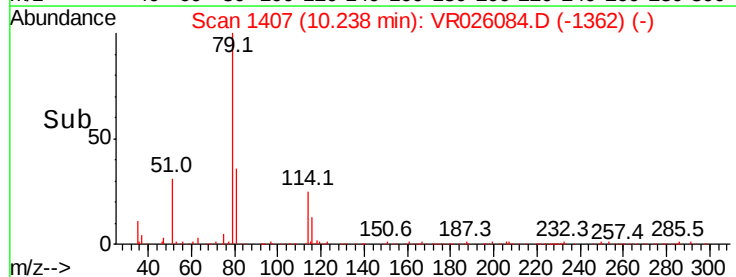
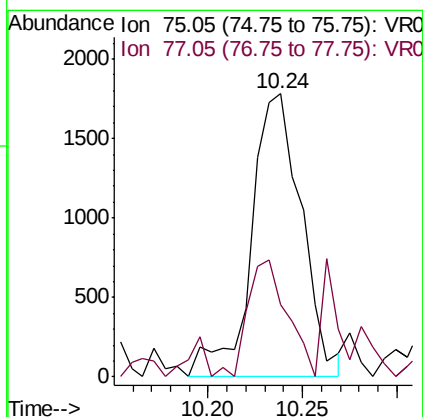
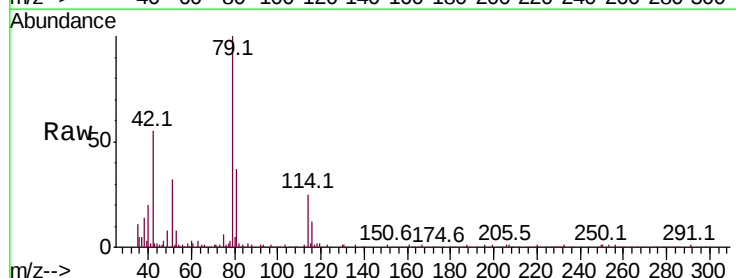


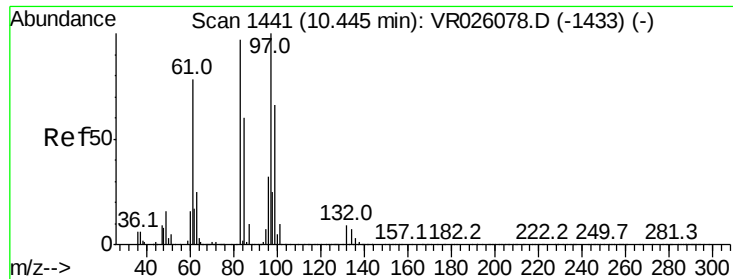

#45
 1,1,2-Trichloroethane
 Concen: 0.547 ug/L
 RT: 10.45 min Scan# 1441
 Delta R.T. -0.00 min
 Lab File: VR026084.D
 Acq: 15 Oct 2018 21:49




Instrument :
 MSVOA_R
 ClientSampleId :


Tot Ion:	97	Resp:	8809
Ion	Ratio	Lower	Upper
97	100		
99	71.0	42.8	79.4
83	91.9	61.9	114.9
85	53.8	39.3	72.9

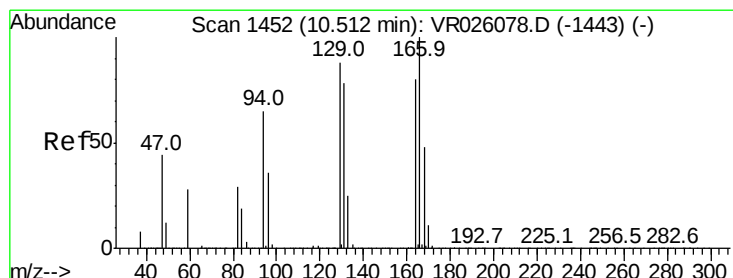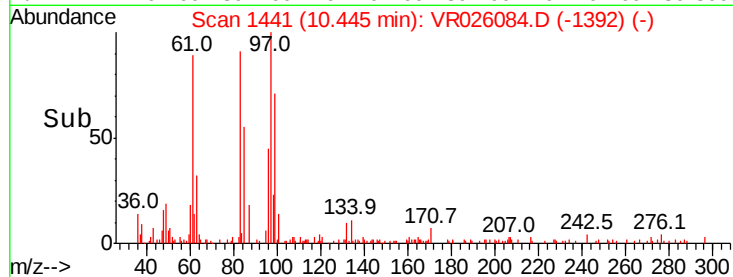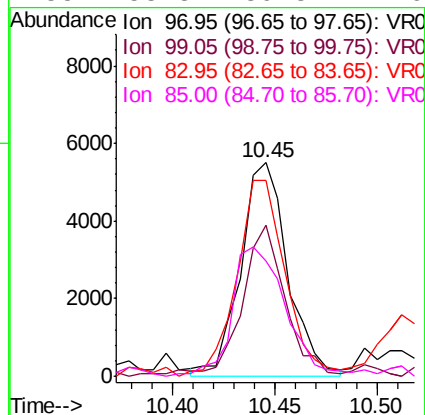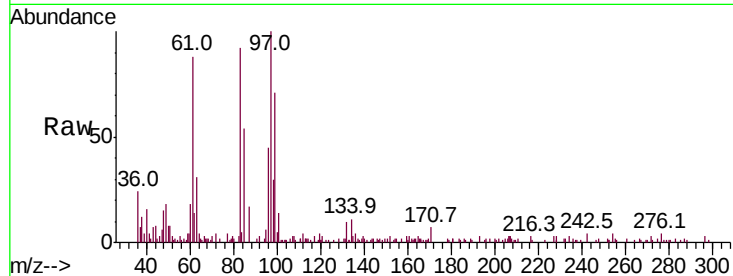

#47
 Tetrachloroethene
 Concen: 1.981 ug/L
 RT: 10.51 min Scan# 1452
 Delta R.T. -0.00 min
 Lab File: VR026084.D
 Acq: 15 Oct 2018 21:49

Tgt Ion:	164	Resp:	65466
Ion	Ratio	Lower	Upper
164	100		
129	100.2	70.3	130.5
131	98.7	67.3	125.1
166	121.5	86.1	159.9


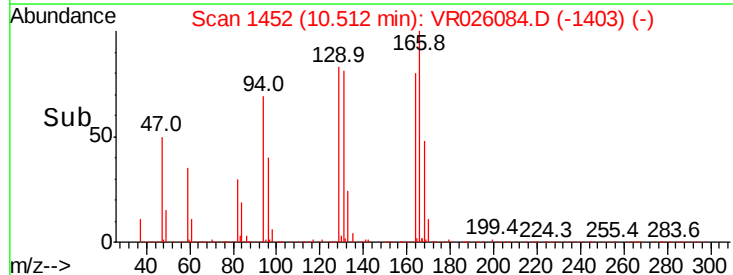
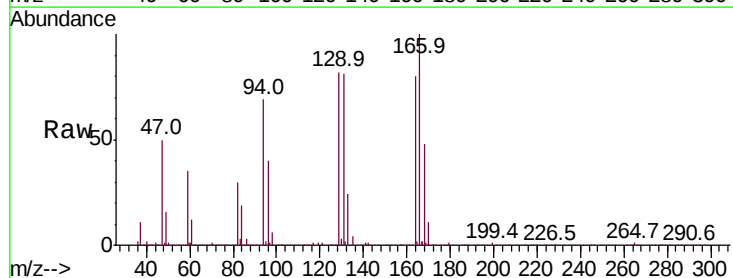
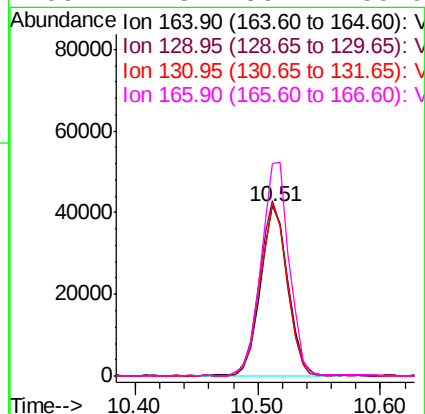


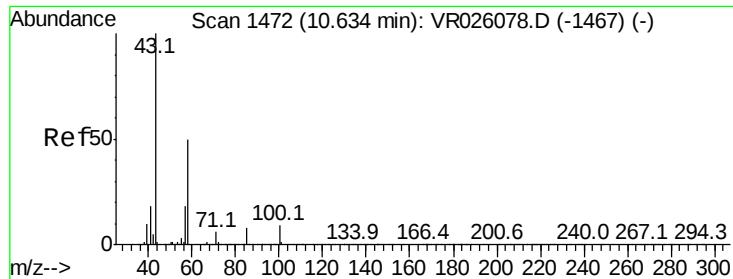

#48
2-Hexanone
Concen: 3.597 ug/L
RT: 10.59 min Scan# 1465
Delta R.T. -0.04 min
Lab File: VR026084.D
Acq: 15 Oct 2018 21:49

Instrument :
MSVOA_R
ClientSampleId :

Tot Ion:	43	Resp:	27374
Ion	Ratio	Lower	Upper
43	100		
58	27.2	39.6	59.4#
57	28.5	14.0	21.0#
100	2.8	7.0	10.6#

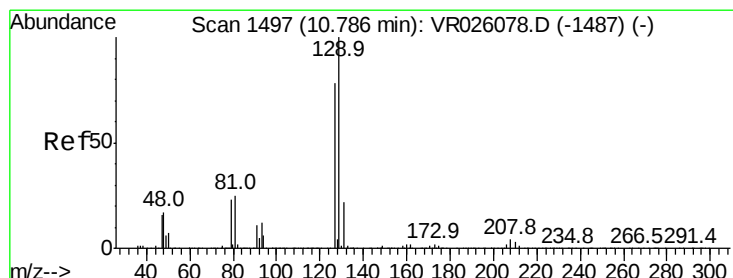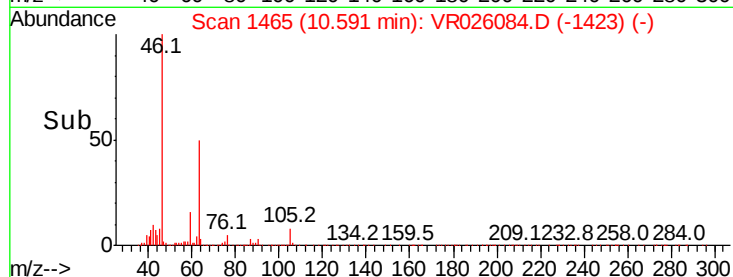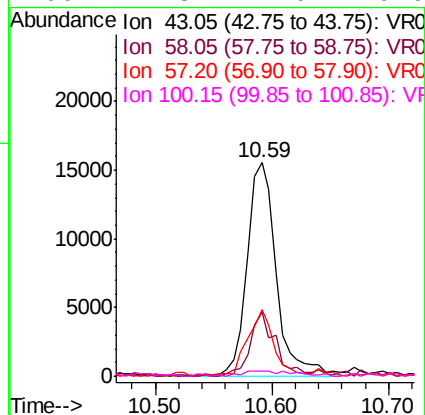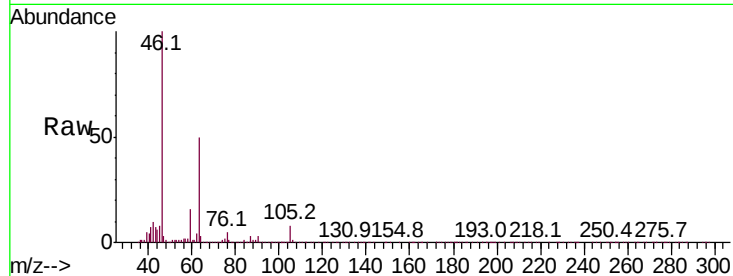

#49
Dibromochloromethane
Concen: 2.995 ug/L
RT: 10.51 min Scan# 1452
Delta R.T. -0.27 min
Lab File: VR026084.D
Acq: 15 Oct 2018 21:49

Tgt Ion:	129	Resp:	54238
Ion	Ratio	Lower	Upper
129	100		
127	0.7	55.0	102.2#

