

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR101918\
Quantitation Report (QT Reviewed)


Data File : VR026149.D
Acq On : 19 Oct 2018 14:37
Operator : SY/MD
Sample : MDL
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL

Manual Integrations
APPROVED

MMDadoda
10/24/2018 12:17:18 PM

Quant Time: Oct 20 02:22:48 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 20 01:53:32 2018
Response via : Initial Calibration

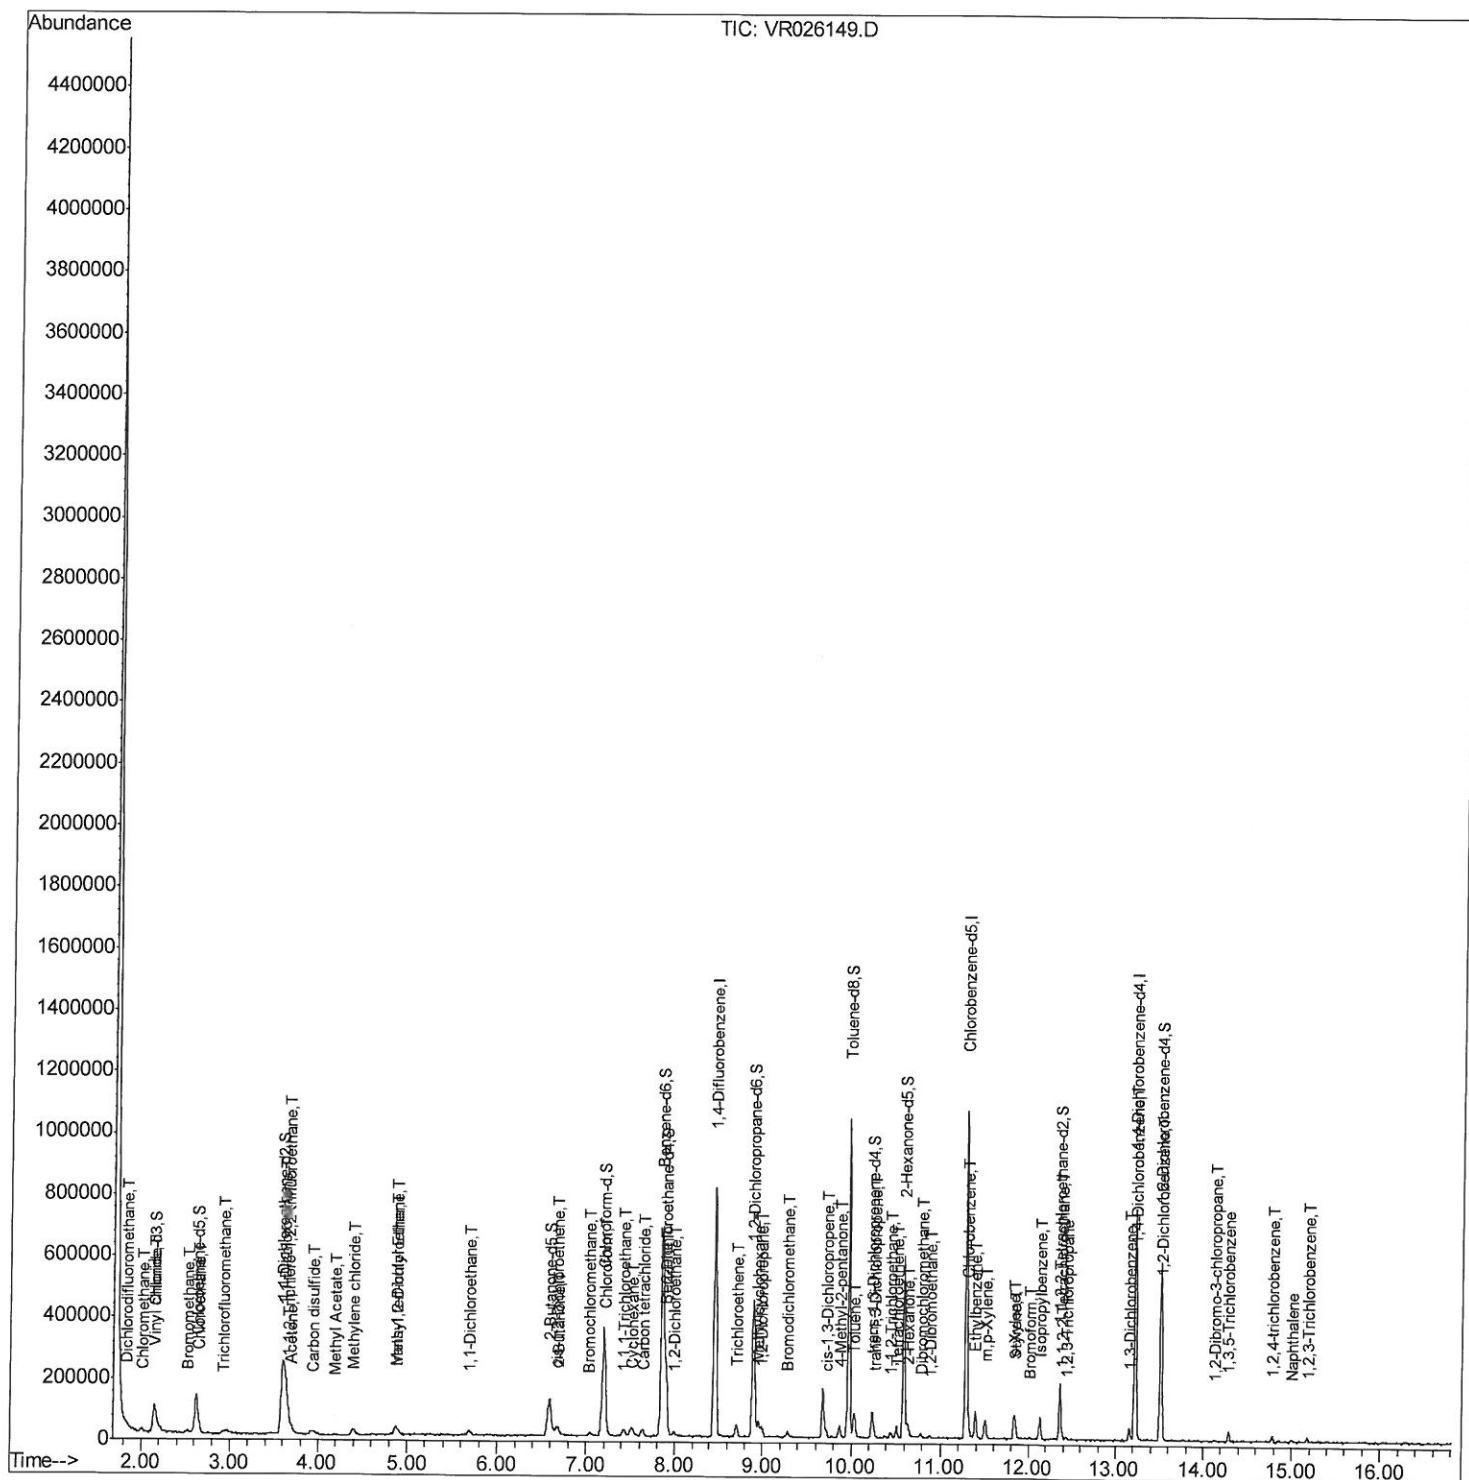

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR101918\
Quantitation Report (Qedit)




Data File : VR026149.D
Acq On : 19 Oct 2018 14:37
Operator : SY/MD
Sample : MDL
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL

Manual Integrations
APPROVED

MMDadoda
10/24/2018 12:17:18 PM

Quant Time: Oct 20 01:59:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 20 01:53:32 2018
Response via : Initial Calibration

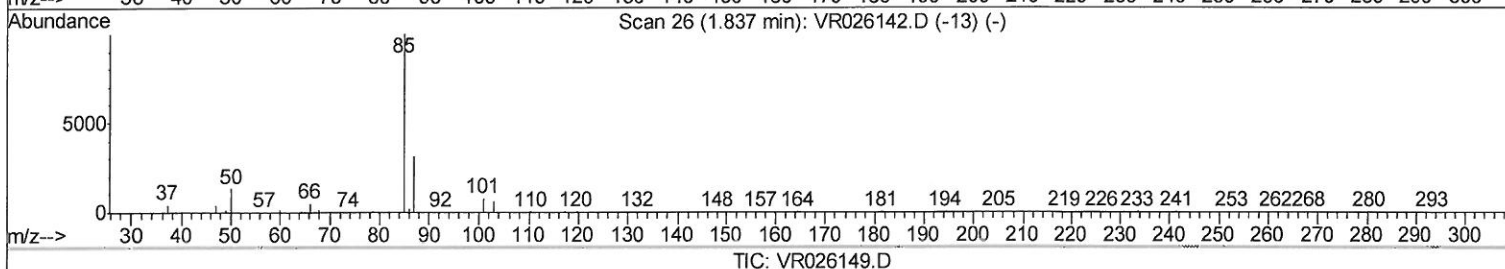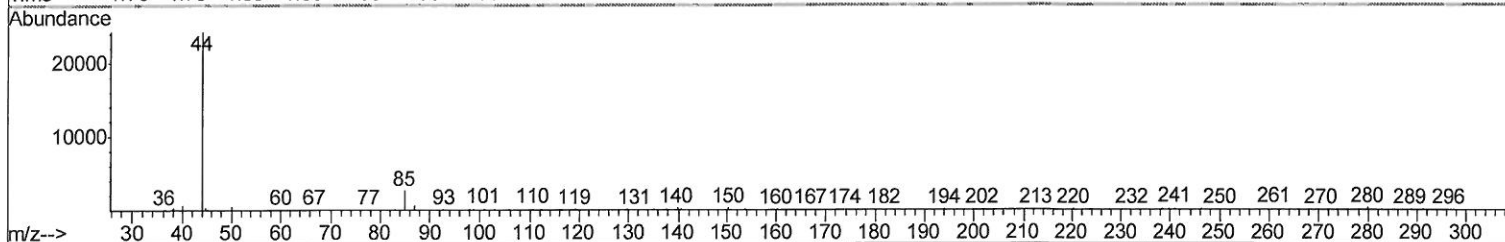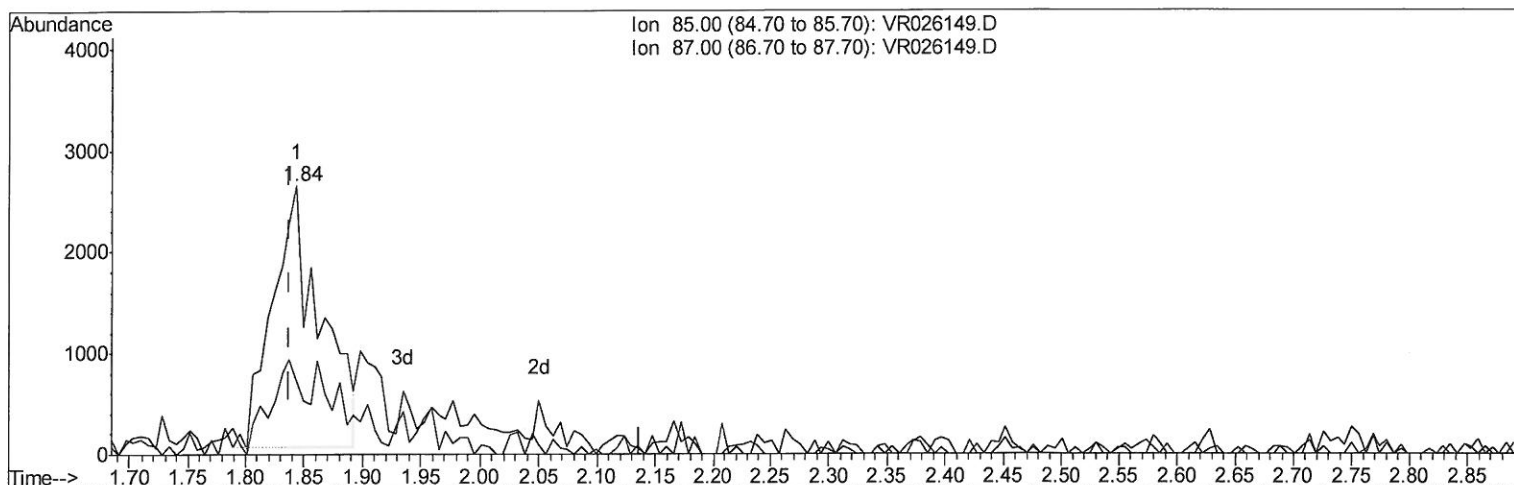

(2) Dichlorodifluoromethane (T)

1.843min (+0.006) 0.20ug/L

response 7261

Ion	Exp%	Act%
85.00	100	100
87.00	29.30	26.11
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR101918\
Quantitation Report (Qedit)




Data File : VR026149.D
Acq On : 19 Oct 2018 14:37
Operator : SY/MD
Sample : MDL
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL

Manual Integrations
APPROVED

MMDadoda
10/24/2018 12:17:18 PM

Quant Time: Oct 20 01:59:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 20 01:53:32 2018
Response via : Initial Calibration

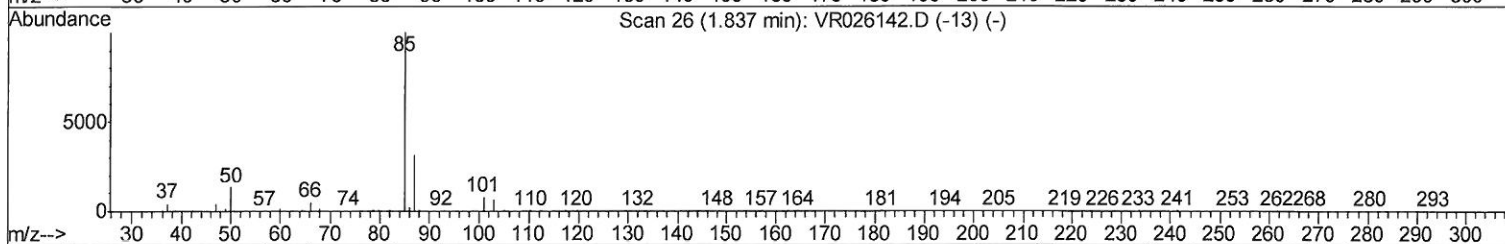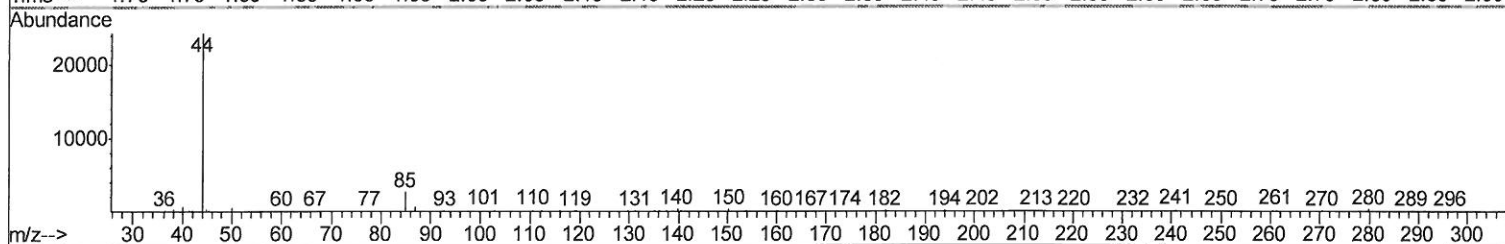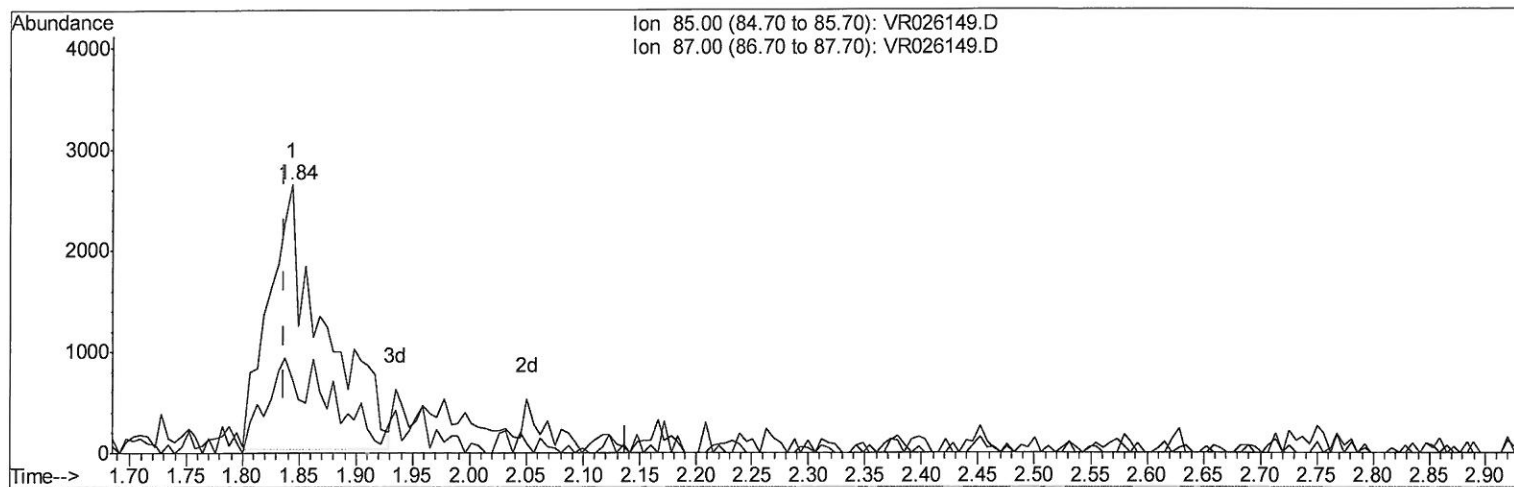

TIC: VR026149.D

(2) Dichlorodifluoromethane (T)

1.843min (+0.006) 0.24ug/L m > 10 { 23 (8 5 }

response 8783

Ion	Exp%	Act%
85.00	100	100
87.00	29.30	21.59#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR101918\
Quantitation Report (Qedit)




Data File : VR026149.D
Acq On : 19 Oct 2018 14:37
Operator : SY/MD
Sample : MDL
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampled :
MDL

Manual Integrations
APPROVED

MMDadoda
10/24/2018 12:17:18 PM

Quant Time: Oct 20 01:59:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 20 01:53:32 2018
Response via : Initial Calibration

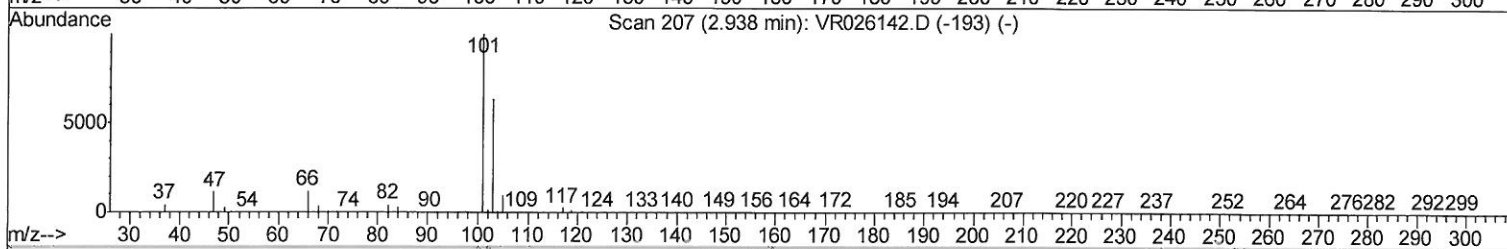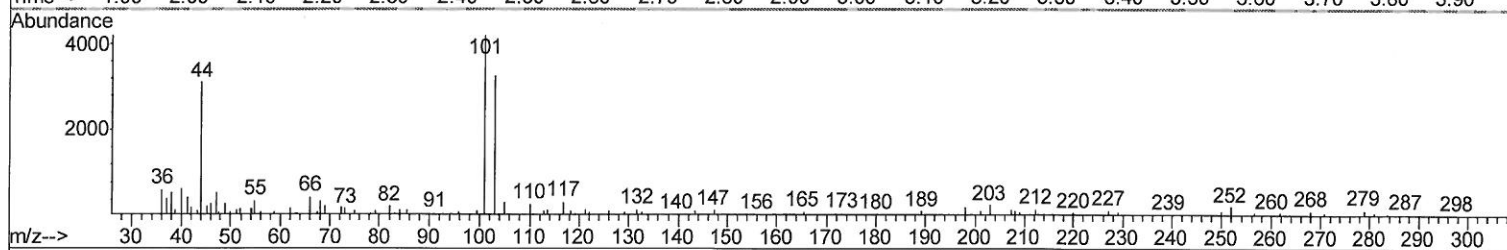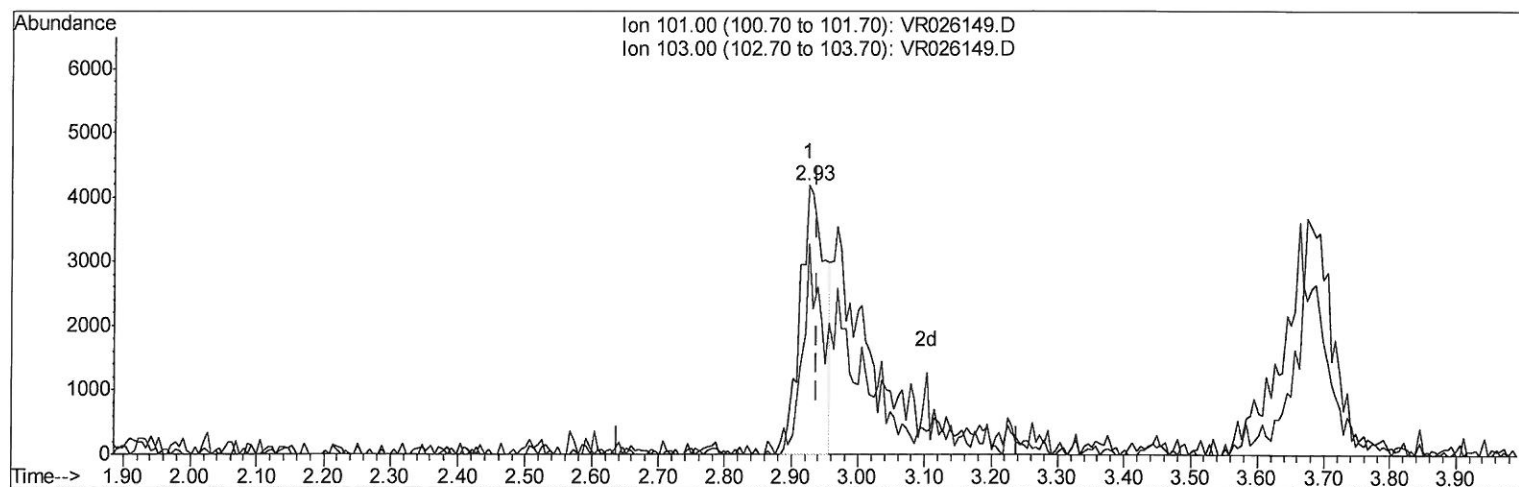

TIC: VR026149.D

(9) Trichlorofluoromethane (T)

2.926min (-0.012) 0.13ug/L

response 10788

Ion	Exp%	Act%
101.00	100	100
103.00	32.50	56.96#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR101918\
Quantitation Report (Qedit)




Data File : VR026149.D
Acq On : 19 Oct 2018 14:37
Operator : SY/MD
Sample : MDL
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampled :
MDL

Manual Integrations
APPROVED

MMDadoda
10/24/2018 12:17:18 PM

Quant Time: Oct 20 01:59:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 20 01:53:32 2018
Response via : Initial Calibration

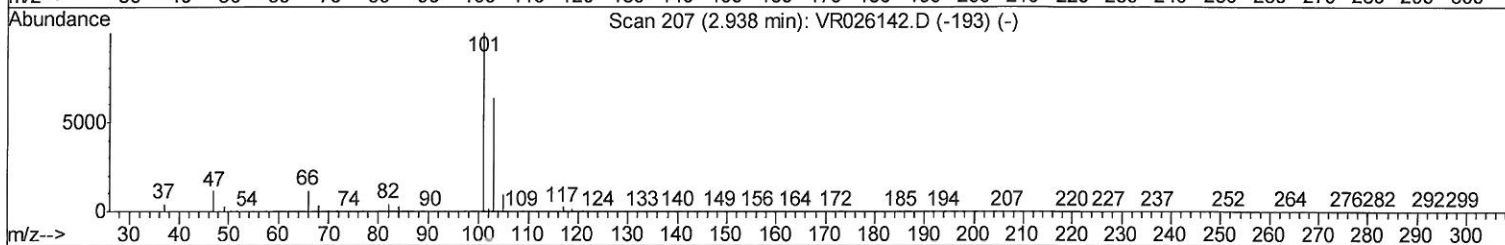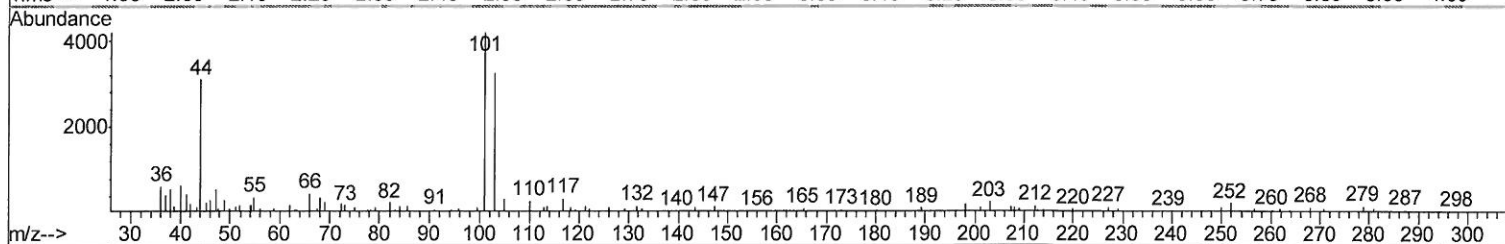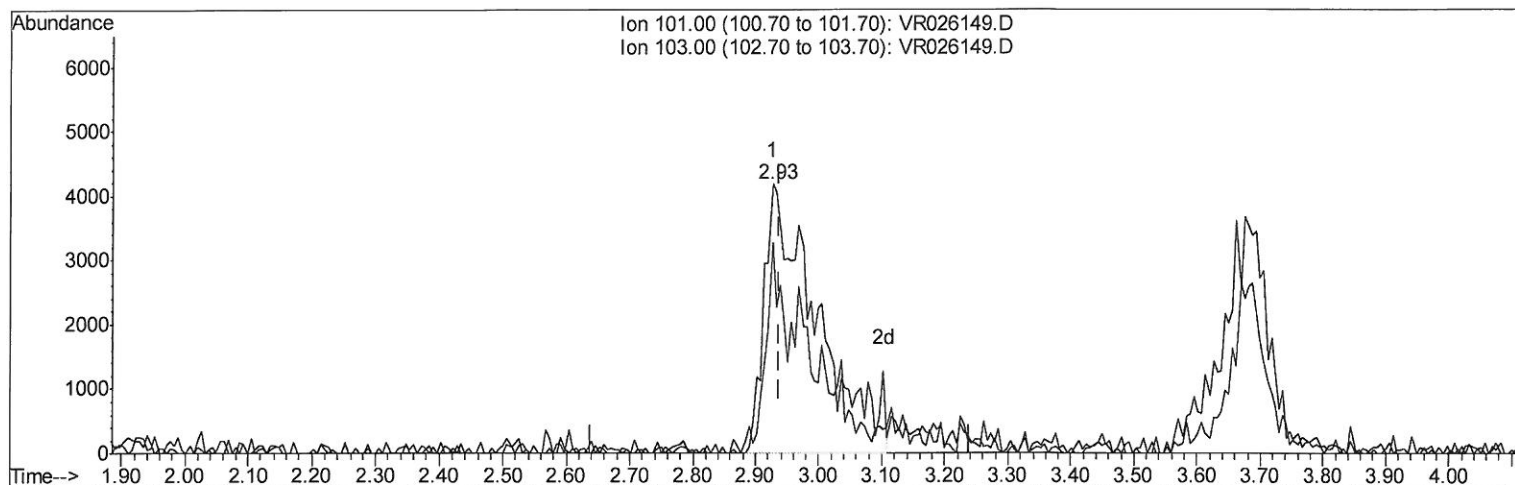

TIC: VR026149.D

(9) Trichlorofluoromethane (T)

2.926min (-0.012) 0.29ug/L m>101201884

response 24160

Ion	Exp%	Act%
101.00	100	100
103.00	32.50	25.43#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR101918\
Quantitation Report (Qedit)




Data File : VR026149.D
Acq On : 19 Oct 2018 14:37
Operator : SY/MD
Sample : MDL
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampled :
MDL

Manual Integrations
APPROVED

MMDadoda
10/24/2018 12:17:18 PM

Quant Time: Oct 20 01:59:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 20 01:53:32 2018
Response via : Initial Calibration

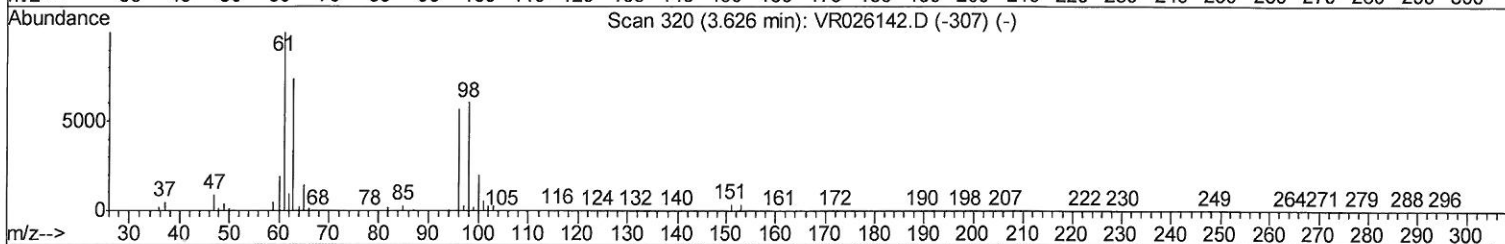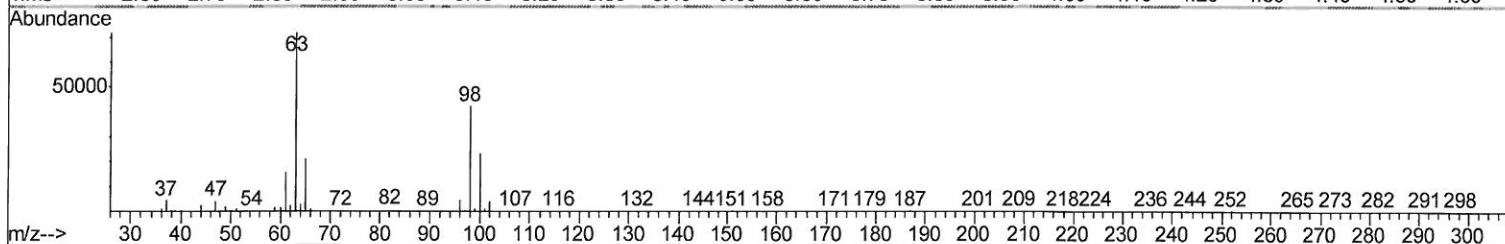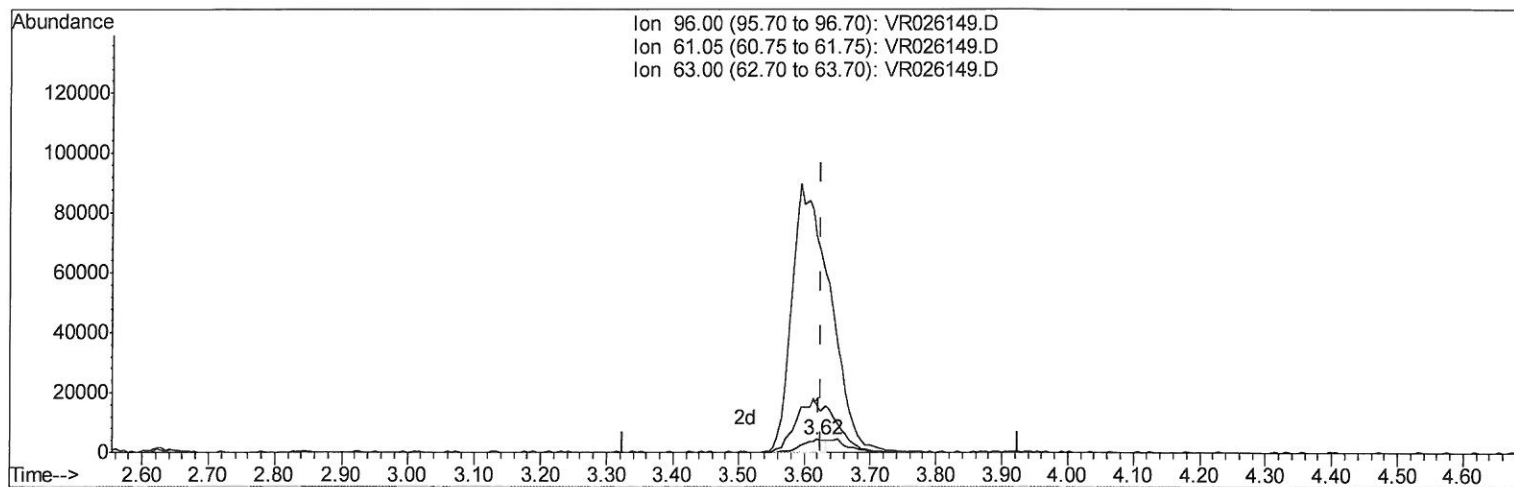

TIC: VR026149.D

(12) 1,1-Dichloroethene (T)

3.620min (-0.006) 0.19ug/L

response 10031

Ion	Exp%	Act%
96.00	100	100
61.05	181.00	355.02#
63.00	178.60	1618.05#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR101918\
Quantitation Report (Qedit)




Data File : VR026149.D
Acq On : 19 Oct 2018 14:37
Operator : SY/MD
Sample : MDL
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL

Manual Integrations
APPROVED

MMDadoda
10/24/2018 12:17:18 PM

Quant Time: Oct 20 01:59:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 20 01:53:32 2018
Response via : Initial Calibration

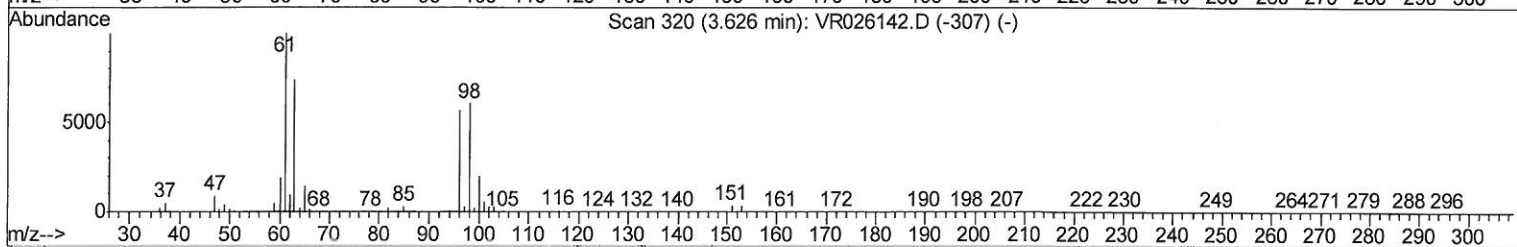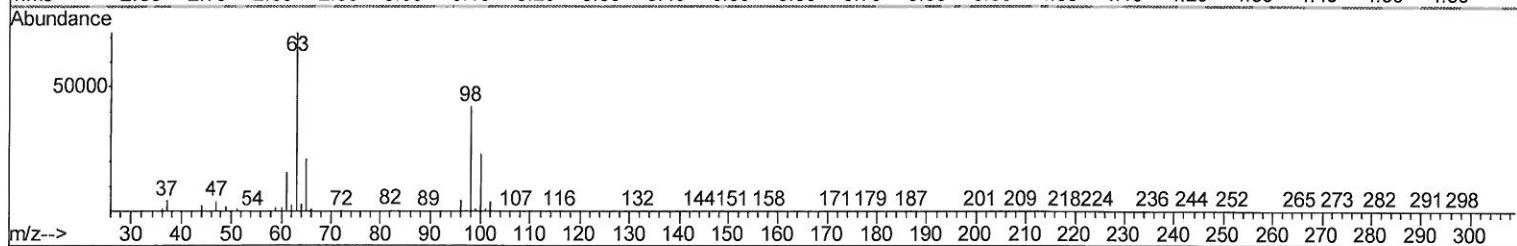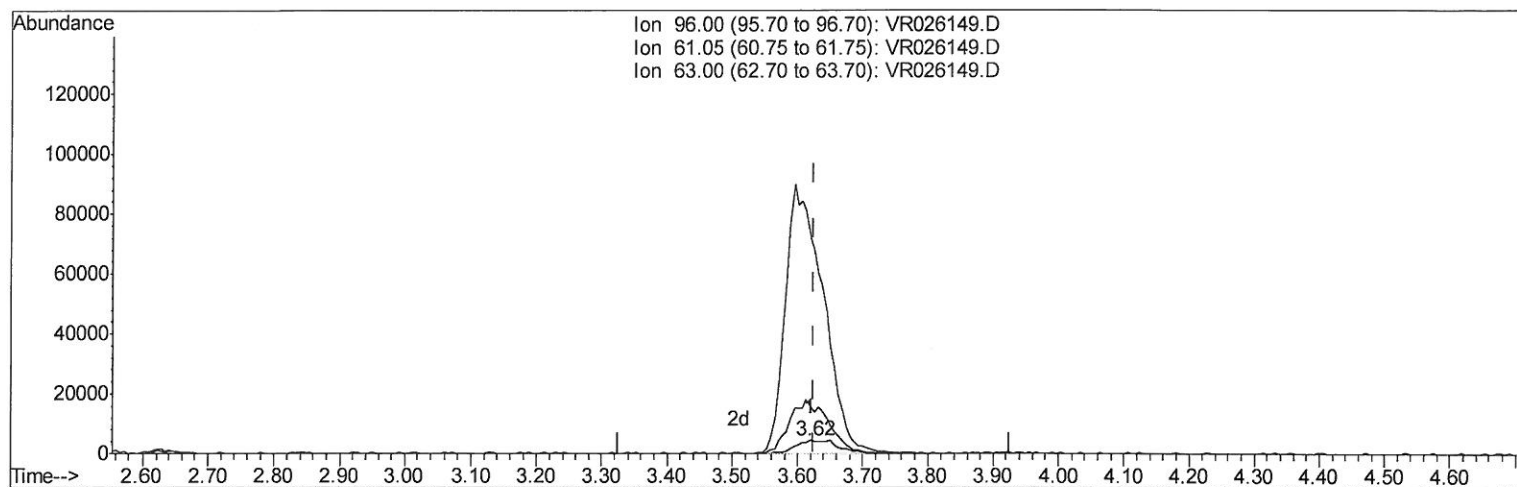

TIC: VR026149.D

(12) 1,1-Dichloroethene (T)

3.620min (-0.006) 0.36ug/L m

10/23/18 sy

response 18984

Ion	Exp%	Act%
96.00	100	100
61.05	181.00	355.02#
63.00	178.60	1618.05#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR101918\
Quantitation Report (Qedit)




Data File : VR026149.D
Acq On : 19 Oct 2018 14:37
Operator : SY/MD
Sample : MDL
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL

Manual Integrations
APPROVED

MMDadoda
10/24/2018 12:17:18 PM

Quant Time: Oct 20 01:59:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 20 01:53:32 2018
Response via : Initial Calibration

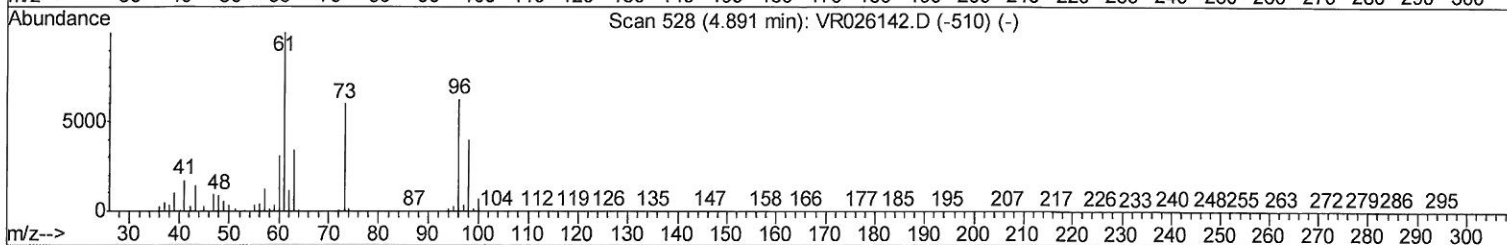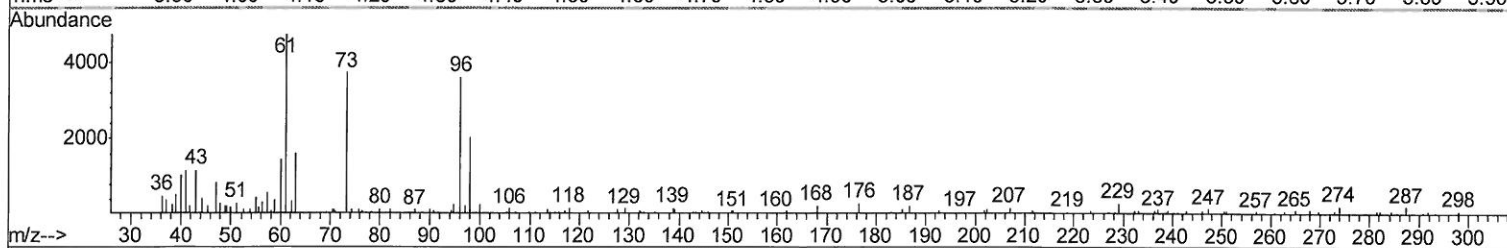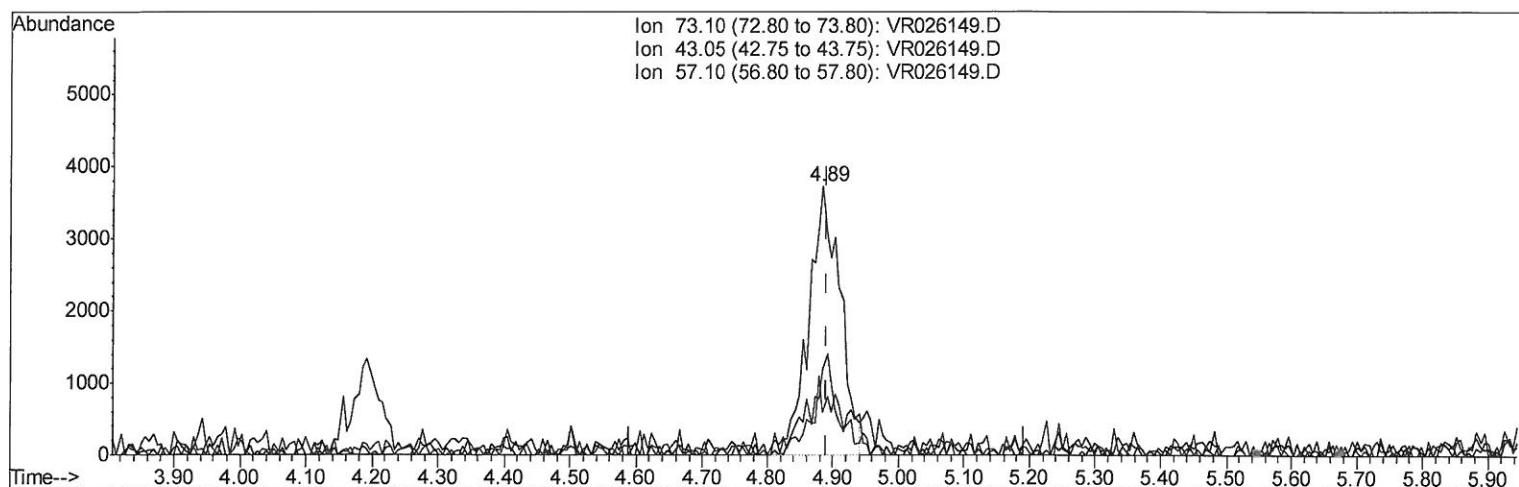

TIC: VR026149.D

(17) Methyl tert-butyl Ether (T)

4.885min (-0.006) 0.25ug/L

response 12257

Ion	Exp%	Act%
73.10	100	100
43.05	25.10	28.69
57.10	23.70	13.39#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR101918\
Quantitation Report (Qedit)




Data File : VR026149.D
Acq On : 19 Oct 2018 14:37
Operator : SY/MD
Sample : MDL
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampled :
MDL

Manual Integrations
APPROVED

MMDadoda
10/24/2018 12:17:18 PM

Quant Time: Oct 20 01:59:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 20 01:53:32 2018
Response via : Initial Calibration

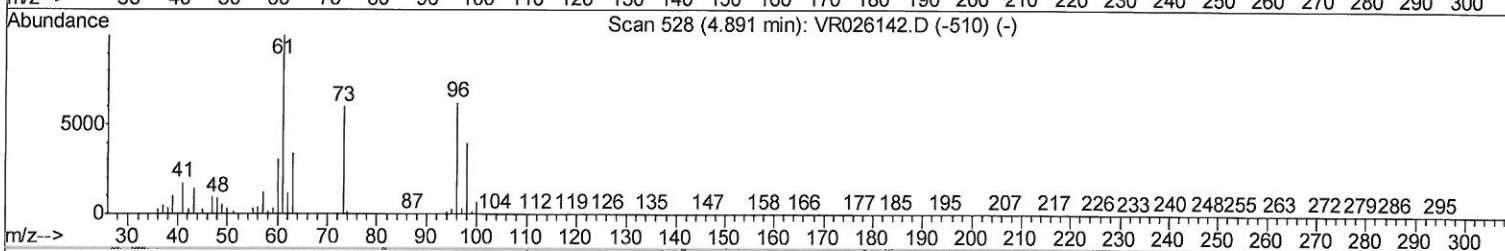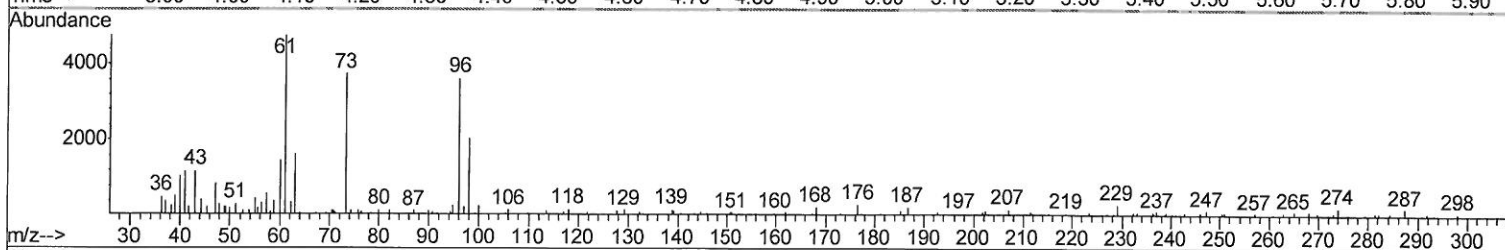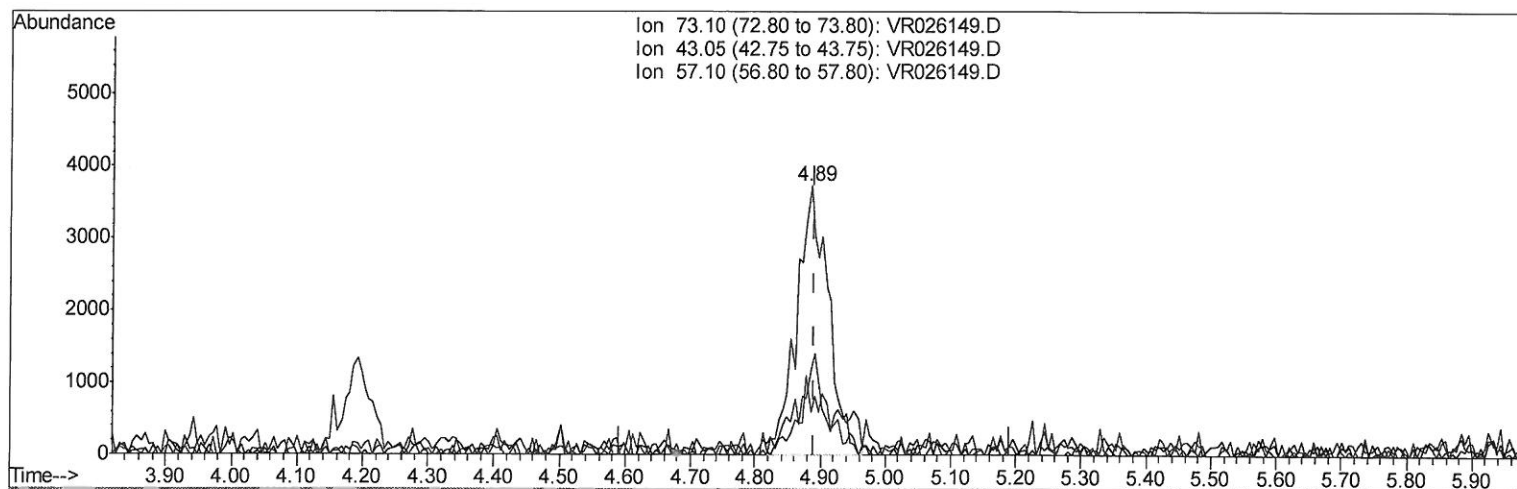

TIC: VR026149.D

(17) Methyl tert-butyl Ether (T)

4.885min (-0.006) 0.27ug/L m

10/23/18 64

response 12853

Ion	Exp%	Act%
73.10	100	100
43.05	25.10	27.36
57.10	23.70	12.77#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR101918\
Quantitation Report (Qedit)




Data File : VR026149.D
Acq On : 19 Oct 2018 14:37
Operator : SY/MD
Sample : MDL
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL

Manual Integrations
APPROVED

MMDadoda
10/24/2018 12:17:18 PM

Quant Time: Oct 20 01:59:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 20 01:53:32 2018
Response via : Initial Calibration

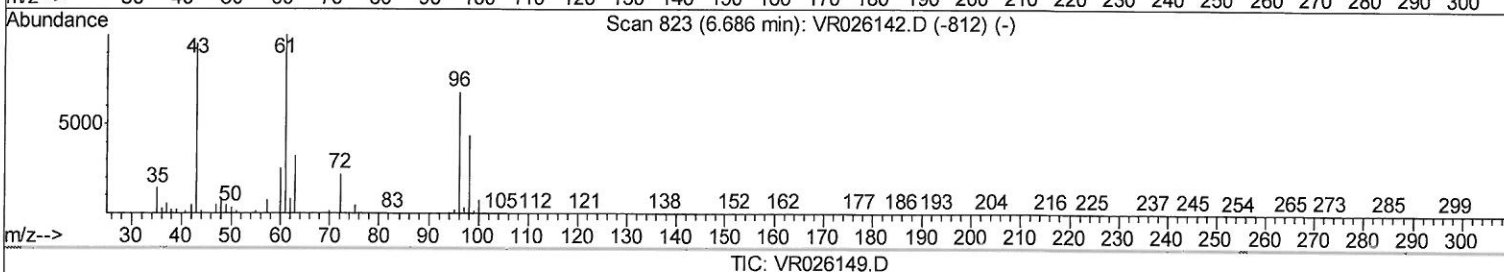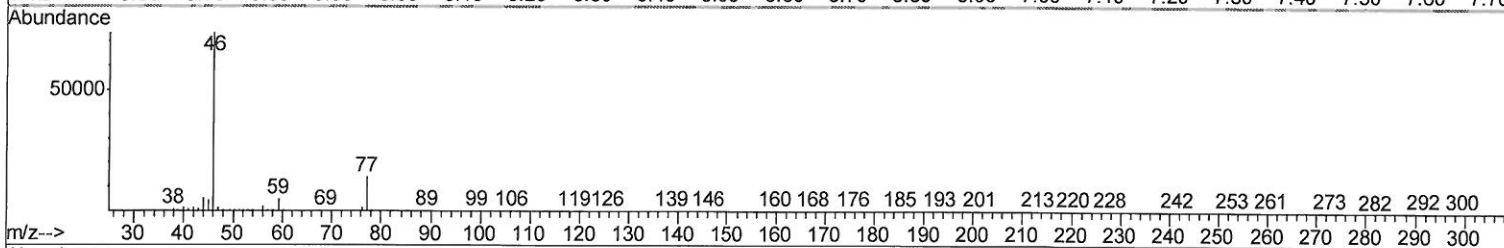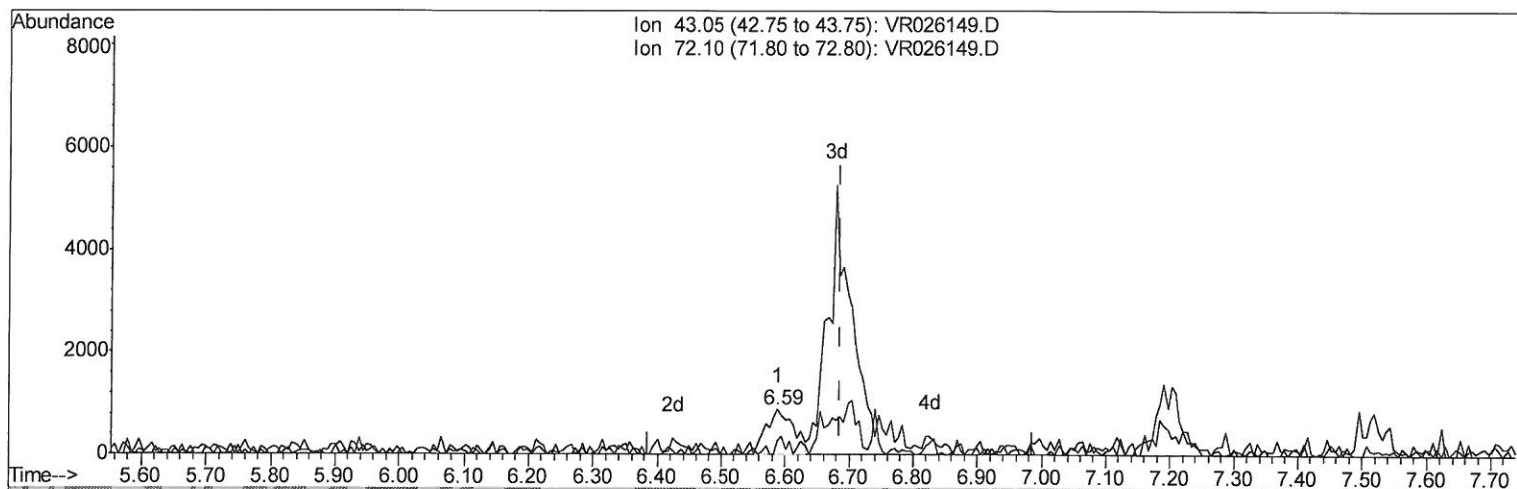

(21) 2-Butanone (T)

6.589min (-0.097) 0.55ug/L

response 2593

Ion	Exp%	Act%
43.05	100	100
72.10	24.50	13.73
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR101918\
Quantitation Report (Qedit)




Data File : VR026149.D
Acq On : 19 Oct 2018 14:37
Operator : SY/MD
Sample : MDL
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL

Manual Integrations
APPROVED

MMDadoda
10/24/2018 12:17:18 PM

Quant Time: Oct 20 01:59:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 20 01:53:32 2018
Response via : Initial Calibration

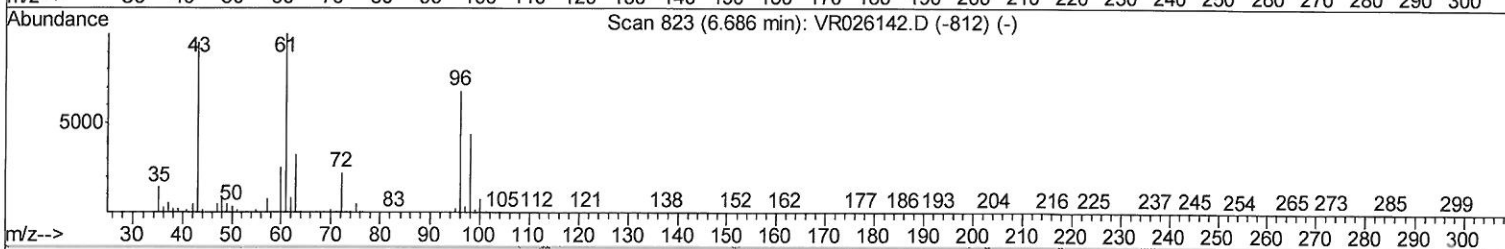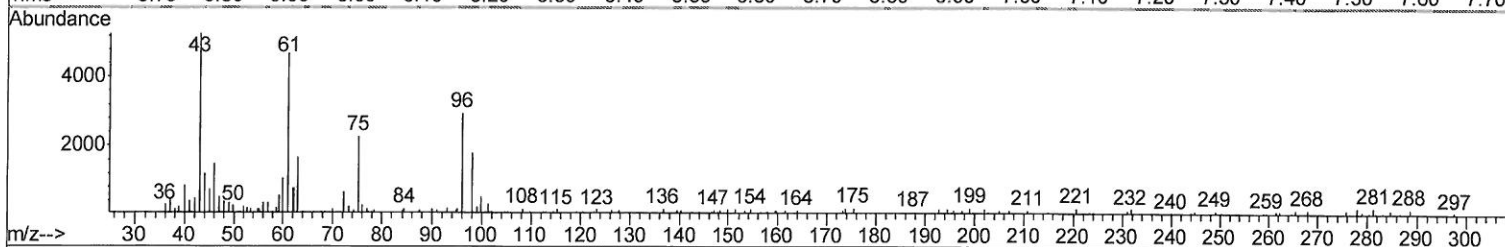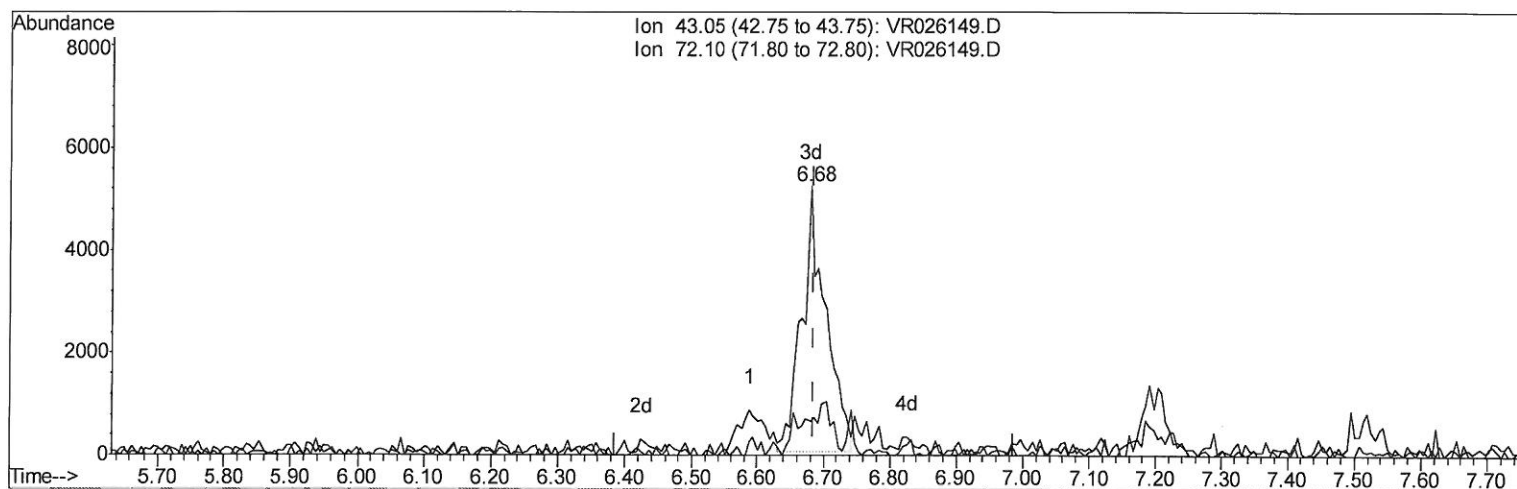

TIC: VR026149.D

(21) 2-Butanone (T)

6.680min (-0.006) 2.77ug/L m

10/23/18 SY

response 12943

Ion	Exp%	Act%
43.05	100	100
72.10	24.50	2.75#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR101918\
Quantitation Report (Qedit)




Data File : VR026149.D
Acq On : 19 Oct 2018 14:37
Operator : SY/MD
Sample : MDL
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL

Manual Integrations
APPROVED

MMDadoda
10/24/2018 12:17:18 PM

Quant Time: Oct 20 01:59:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 20 01:53:32 2018
Response via : Initial Calibration

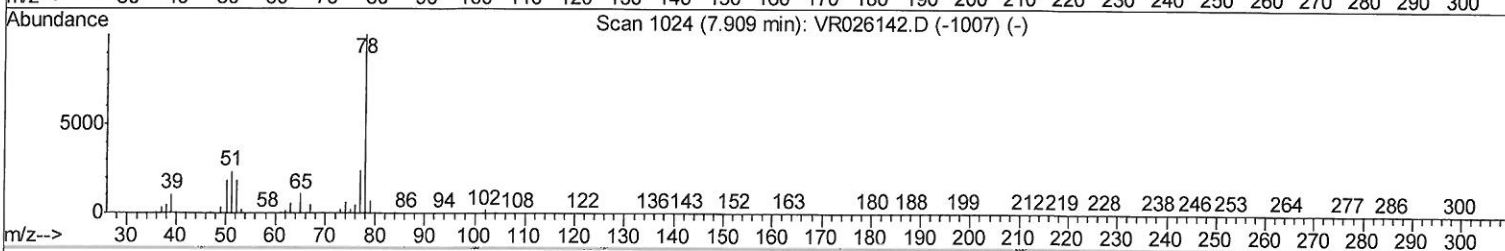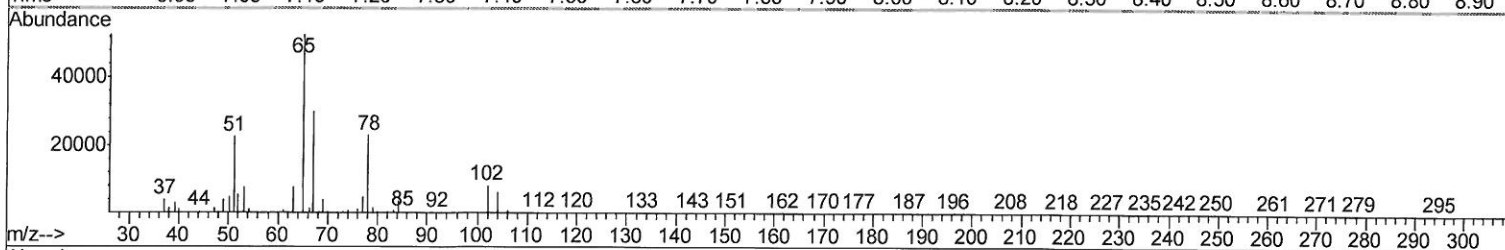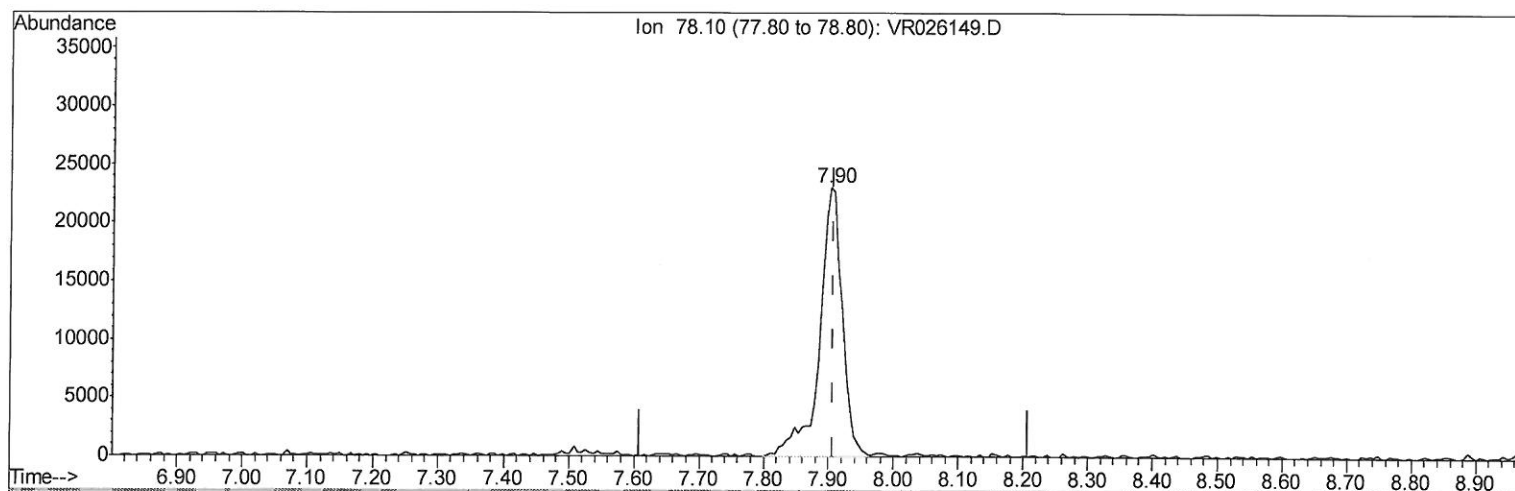

TIC: VR026149.D

(33) Benzene (T)

7.903min (-0.006) 0.32ug/L

response 56332

Ion	Exp%	Act%
78.10	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR101918\
Quantitation Report (Qedit)




Data File : VR026149.D
Acq On : 19 Oct 2018 14:37
Operator : SY/MD
Sample : MDL
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL

Manual Integrations
APPROVED

MMDadoda
10/24/2018 12:17:18 PM

Quant Time: Oct 20 01:59:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 20 01:53:32 2018
Response via : Initial Calibration

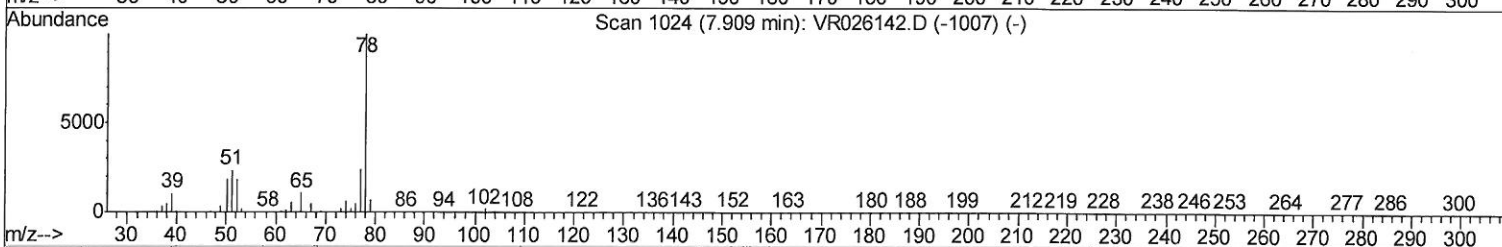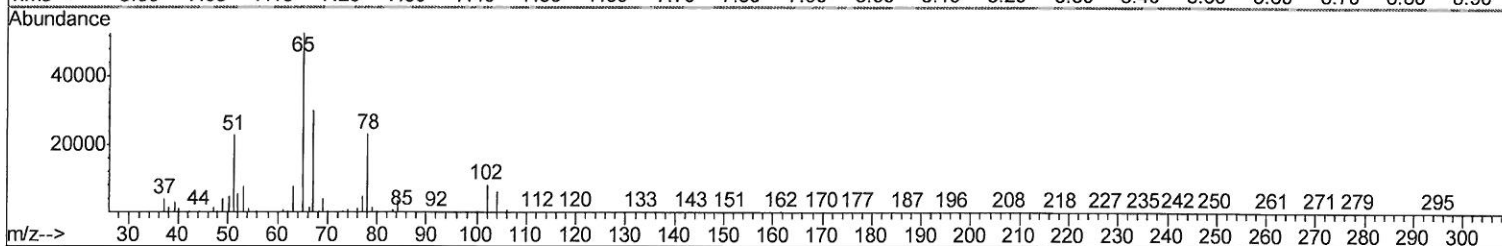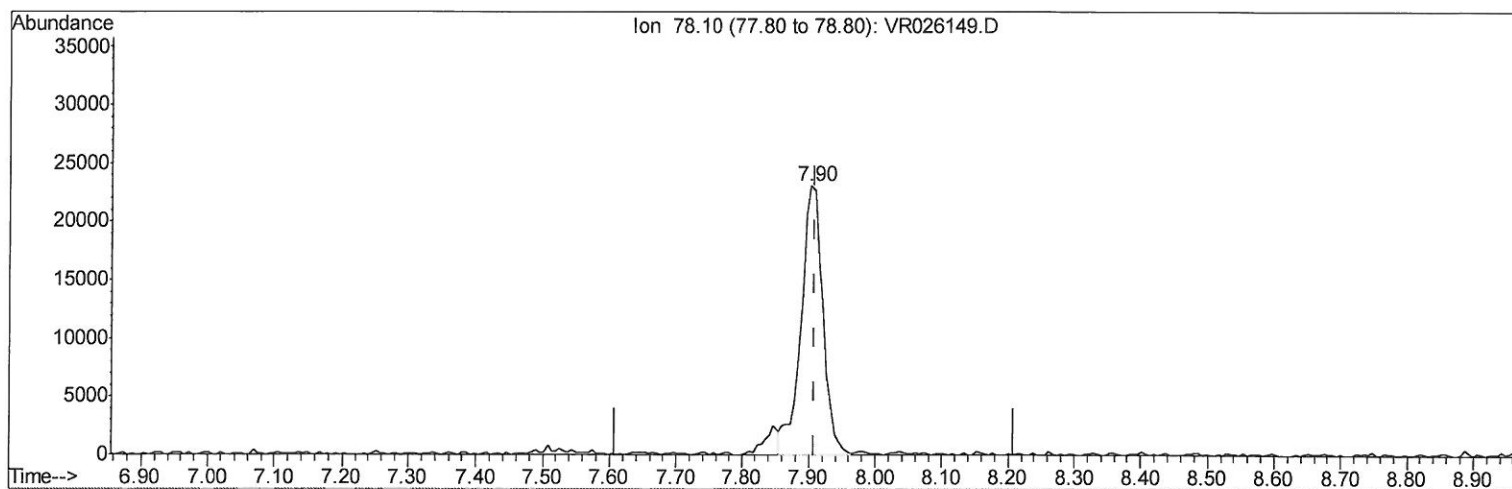

TIC: VR026149.D

(33) Benzene (T)

7.903min (-0.006) 0.30ug/L m

10/23/18

response 52665

Ion	Exp%	Act%
78.10	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR101918\
Quantitation Report (Qedit)




Data File : VR026149.D
Acq On : 19 Oct 2018 14:37
Operator : SY/MD
Sample : MDL
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
MDL

Manual Integrations
APPROVED

MMDadoda
10/24/2018 12:17:18 PM

Quant Time: Oct 20 01:59:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 20 01:53:32 2018
Response via : Initial Calibration

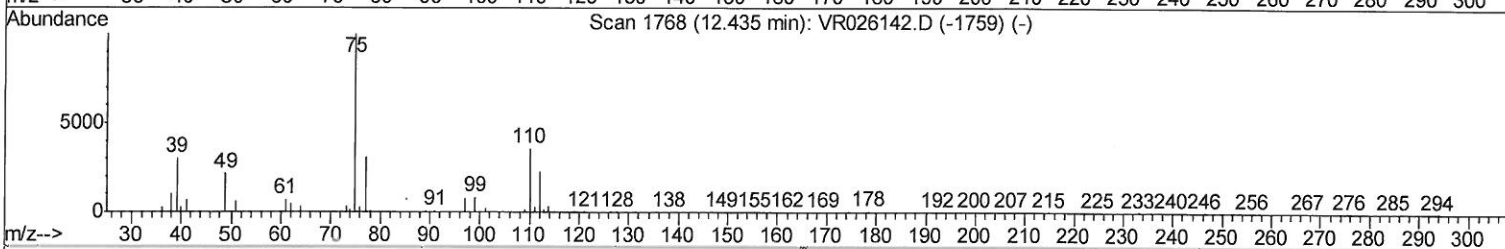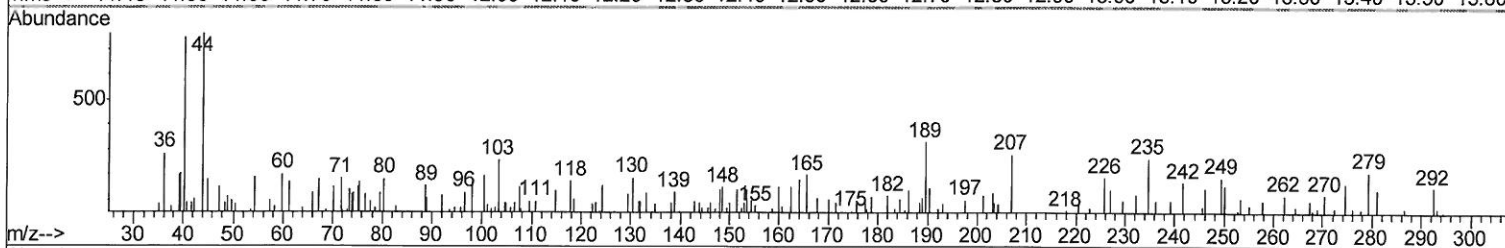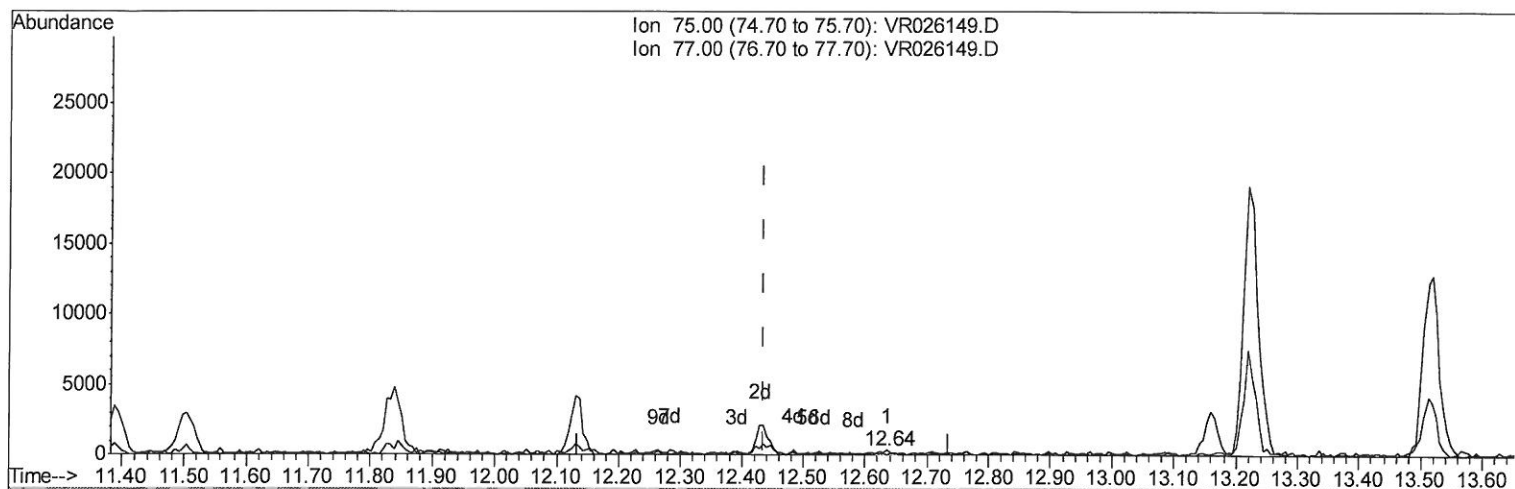

TIC: VR026149.D

(59) 1,2,3-Trichloropropane

12.636min (+0.201) 0.03ug/L

response 346

Ion	Exp%	Act%
75.00	100	100
77.00	32.70	33.53
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR101918\
Quantitation Report (Qedit)




Data File : VR026149.D
Acq On : 19 Oct 2018 14:37
Operator : SY/MD
Sample : MDL
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampled :
MDL

Manual Integrations
APPROVED

MMDadoda
10/24/2018 12:17:18 PM

Quant Time: Oct 20 01:59:09 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 20 01:53:32 2018
Response via : Initial Calibration

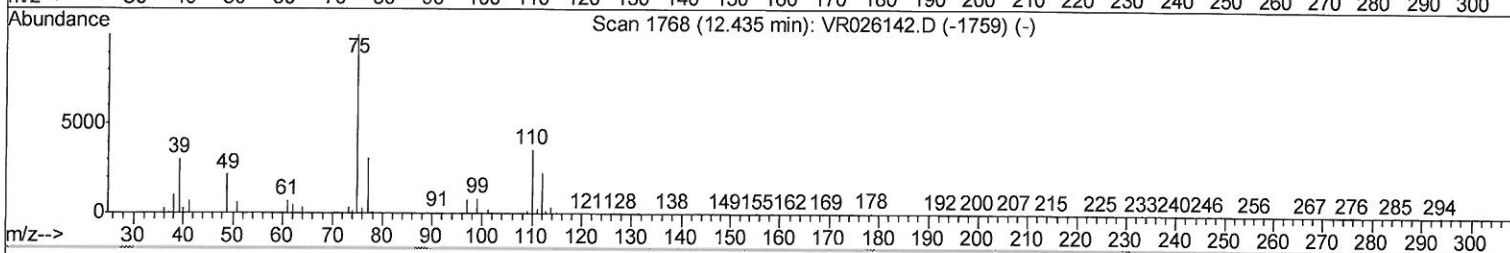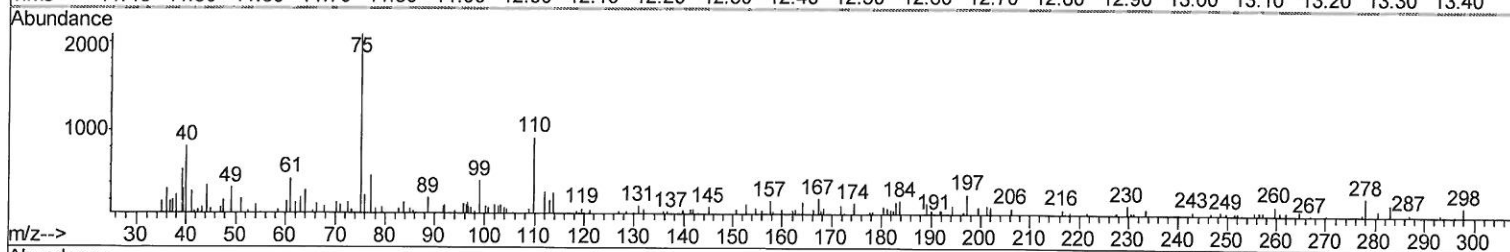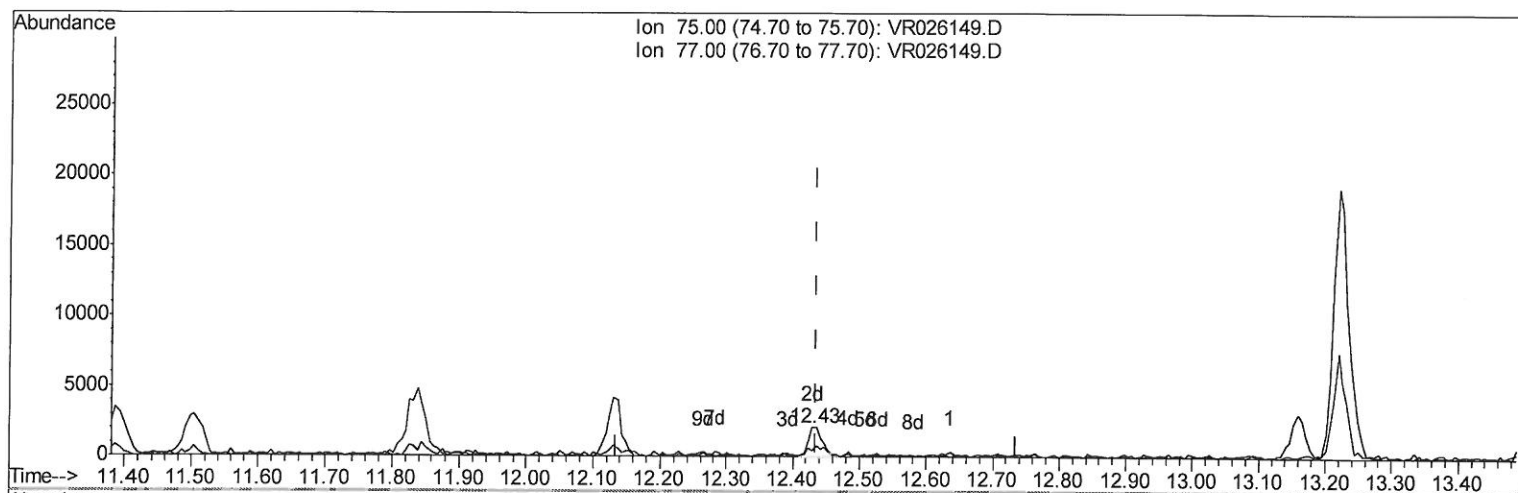

TIC: VR026149.D

(59) 1,2,3-Trichloropropane

12.429min (-0.006) 0.27ug/L m

10/23/18 SY

response 3064

Ion	Exp%	Act%
75.00	100	100
77.00	32.70	3.79#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR101918\
Quantitation Report (QT Reviewed)

Data File : VR026149.D
Acq On : 19 Oct 2018 14:37
Operator : SY/MD
Sample : MDL
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampled :
MDL

Manual Integrations
APPROVED

MMDadoda
10/24/2018 12:17:18 PM

Quant Time: Oct 20 02:22:48 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 20 01:53:32 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	545240	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	463116	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	146960	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.15	65	177743	3.72	ug/L	-0.01
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.40%
7) Chloroethane-d5	2.63	69	186408	4.54	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.80%
11) 1,1-Dichloroethene-d2	3.60	63	361011	3.08	ug/L	-0.01
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.60%
20) 2-Butanone-d5	6.59	46	225036	57.44	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.88%
24) Chloroform-d	7.20	84	344942	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.00%
26) 1,2-Dichloroethane-d4	7.89	65	147929	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.80%
32) Benzene-d6	7.85	84	660087	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.80%
36) 1,2-Dichloropropane-d6	8.90	67	190208	4.95	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.00%
41) Toluene-d8	9.97	98	582926	4.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.00%
43) trans-1,3-Dichloropropene-	10.24	79	37815	3.75	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.00%
46) 2-Hexanone-d5	10.59	63	166847	57.33	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	114.66%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	76966	5.10	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.00%
64) 1,2-Dichlorobenzene-d4	13.52	152	114021	4.91	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.20%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	1.84	85	8783m	0.240	ug/L	
3) Chloromethane	2.01	50	17517	0.301	ug/L	88
5) Vinyl chloride	2.15	62	17202	0.297	ug/L #	79
6) Bromomethane	2.53	94	10942	0.286	ug/L	82
8) Chloroethane	2.65	64	10126	0.282	ug/L	86
9) Trichlorofluoromethane	2.93	101	24160m	0.289	ug/L	
10) 1,1,2-Trichloro-1,2,2-trif	3.67	101	18172	0.364	ug/L	88
12) 1,1-Dichloroethene	3.62	96	18984m	0.358	ug/L	
13) Acetone	3.69	43	12975	3.204	ug/L	68
14) Carbon disulfide	3.94	76	33350	0.241	ug/L #	94
15) Methyl Acetate	4.19	43	3469	0.328	ug/L #	81
16) Methylene chloride	4.40	84	18400	0.383	ug/L	91
17) Methyl tert-butyl Ether	4.89	73	12853m	0.267	ug/L	
18) trans-1,2-Dichloroethene	4.88	96	10815	0.270	ug/L	84
19) 1,1-Dichloroethane	5.69	63	20540	0.273	ug/L	90
21) 2-Butanone	6.68	43	12943m	2.770	ug/L	
22) cis-1,2-Dichloroethene	6.67	96	10131	0.267	ug/L #	94

10/23/18

10/23/18

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR101918\
Quantitation Report (QT Reviewed)

Data File : VR026149.D
Acq On : 19 Oct 2018 14:37
Operator : SY/MD
Sample : MDL
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampled :
MDL

Manual Integrations
APPROVED

MMDadoda
10/24/2018 12:17:18 PM

Quant Time: Oct 20 02:22:48 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 20 01:53:32 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
23) Bromochloromethane	7.03	128	3691	0.347	ug/L #	68
25) Chloroform	7.22	83	21362	0.291	ug/L	91
27) 1,2-Dichloroethane	7.99	62	11037	0.307	ug/L #	80
29) 1,1,1-Trichloroethane	7.42	97	16513	0.261	ug/L	91
30) Cyclohexane	7.53	56	13073	0.206	ug/L	96
31) Carbon tetrachloride	7.64	117	14830	0.258	ug/L	99
33) Benzene	7.90	78	52665m	0.303	ug/L	10/23/18 24
34) Trichloroethene	8.71	95	12440	0.280	ug/L	87
35) Methylcyclohexane	8.95	83	13128	0.198	ug/L #	76
37) 1,2-Dichloropropane	8.99	63	10751	0.293	ug/L #	94
38) Bromodichloromethane	9.28	83	10154	0.258	ug/L	80
39) cis-1,3-Dichloropropene	9.72	75	10869	0.259	ug/L	88
40) 4-Methyl-2-pentanone	9.87	43	24886	2.223	ug/L #	91
42) Toluene	10.03	91	48048	0.262	ug/L	92
44) trans-1,3-Dichloropropene	10.26	75	9429	0.322	ug/L	86
45) 1,1,2-Trichloroethane	10.43	97	3664	0.237	ug/L	83
47) Tetrachloroethene	10.51	164	7584	0.239	ug/L	89
48) 2-Hexanone	10.64	43	22573	3.087	ug/L #	83
49) Dibromochloromethane	10.78	129	4006	0.230	ug/L	96
50) 1,2-Dibromoethane	10.88	107	3500	0.262	ug/L #	85
51) Chlorobenzene	11.31	112	27660	0.272	ug/L	96
52) Ethylbenzene	11.39	91	49128	0.233	ug/L	94
53) m,p-Xylene	11.50	106	16262	0.212	ug/L	89
54) o-Xylene	11.83	106	13697	0.194	ug/L	78
55) Styrene	11.84	104	19289	0.178	ug/L	91
56) Isopropylbenzene	12.13	105	37069	0.189	ug/L	96
58) 1,1,2,2-Tetrachloroethane	12.39	83	4586	0.292	ug/L #	80
59) 1,2,3-Trichloropropane	12.43	75	3064m	0.266	ug/L	10/23/18
61) Bromoform	12.00	173	1161	0.227	ug/L #	91
62) 1,3-Dichlorobenzene	13.16	146	11745	0.241	ug/L	93
63) 1,4-Dichlorobenzene	13.24	146	14788	0.292	ug/L	91
65) 1,2-Dichlorobenzene	13.53	146	12262	0.313	ug/L	87
66) 1,2-Dibromo-3-chloropropan	14.14	75	408	0.256	ug/L #	76
67) 1,3,5-Trichlorobenzene	14.29	180	7672	0.258	ug/L	95
68) 1,2,4-trichlorobenzene	14.79	180	4149	0.239	ug/L	90
69) Naphthalene	15.00	128	4137	0.245	ug/L #	89
70) 1,2,3-Trichlorobenzene	15.18	180	3192	0.265	ug/L #	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed