
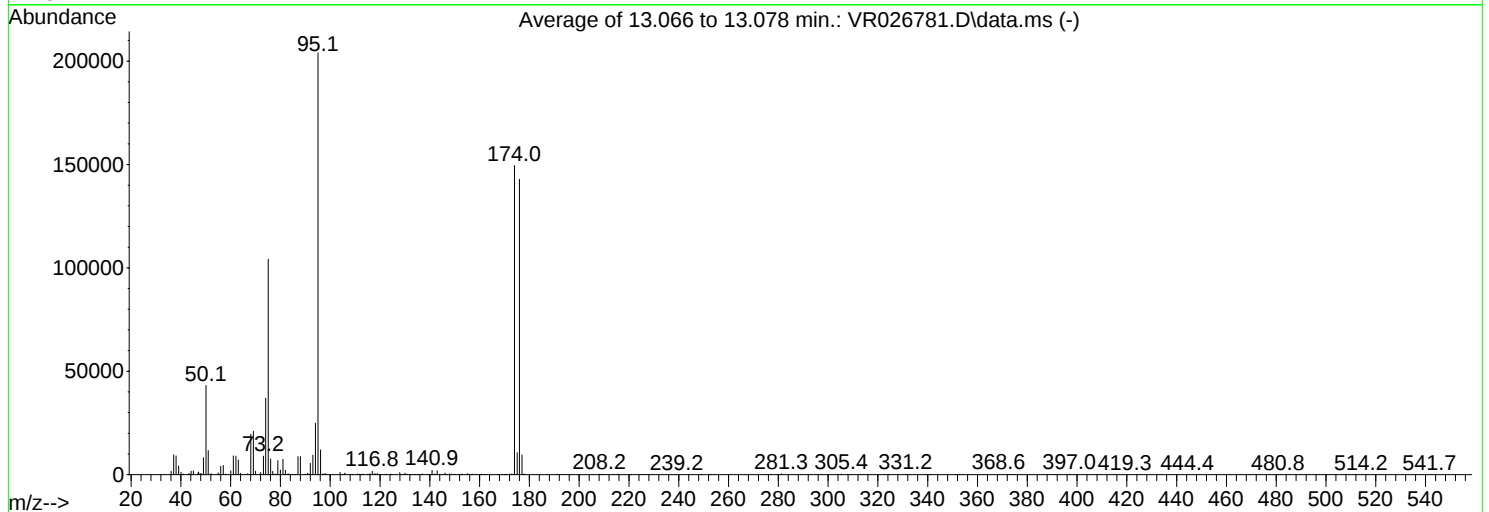


Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR102225\
Data File : VR026781.D
Acq On : 22 Oct 2025 9:59
Operator : SY/MD
Sample : BFB
Misc : 5mL/MSVOA_R/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_R\methods\82R102225W.M
Title : SW846 8260
Last Update : Fri Oct 24 09:26:03 2025

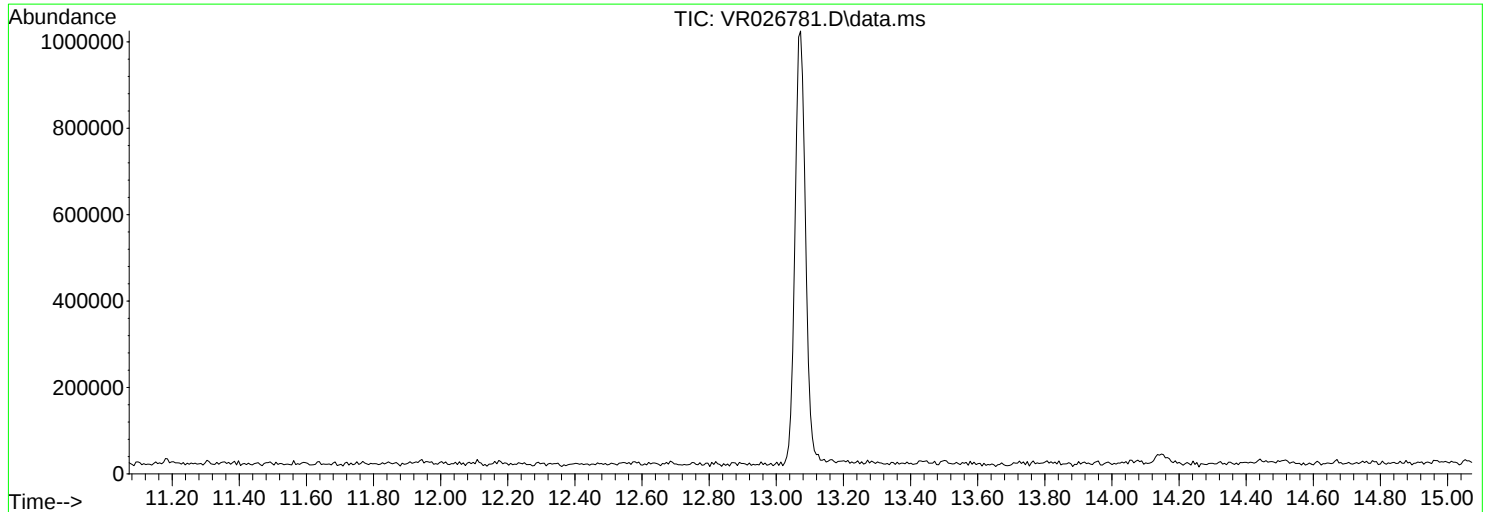

AutoFind: Scans 1904, 1905, 1906; Background Corrected with Scan 1894

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	43120	PASS
75	95	30	60	51.1	104232	PASS
95	95	100	100	100.0	204011	PASS
96	95	5	9	5.9	11969	PASS
173	174	0.00	2	0.2	348	PASS
174	95	50	100	73.3	149525	PASS
175	174	5	9	7.1	10641	PASS
176	174	95	101	95.5	142848	PASS
177	176	5	9	6.6	9497	PASS